

Sample Name : β -Endorphin, human
 Cat No. : RP11344
 Lot No. : PE8431902
 Time Processed : 2:42:50
 Month-Day-Year Processed : 03/01/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK12010012

<Chromatogram>

mV

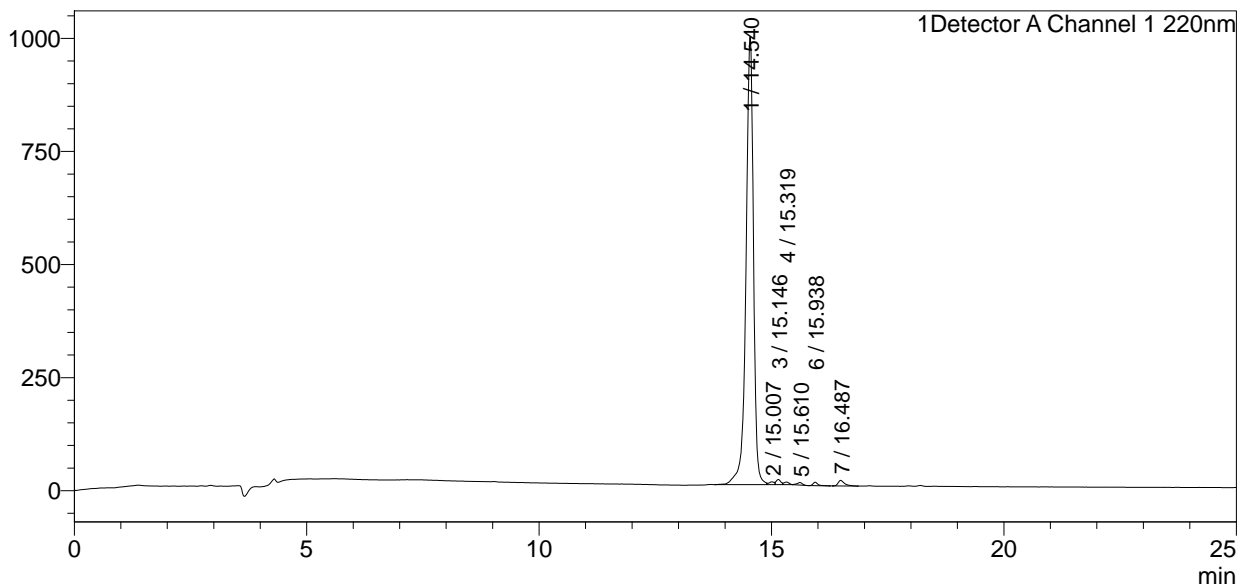

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.540	11019759	990649	96.646
2	15.007	48784	6023	0.428
3	15.146	76510	11238	0.671
4	15.319	40857	5529	0.358
5	15.610	44029	5605	0.386
6	15.938	55009	7715	0.482
7	16.487	117298	12289	1.029
Total		11402246	1039049	100.000