


Mass Spectrum

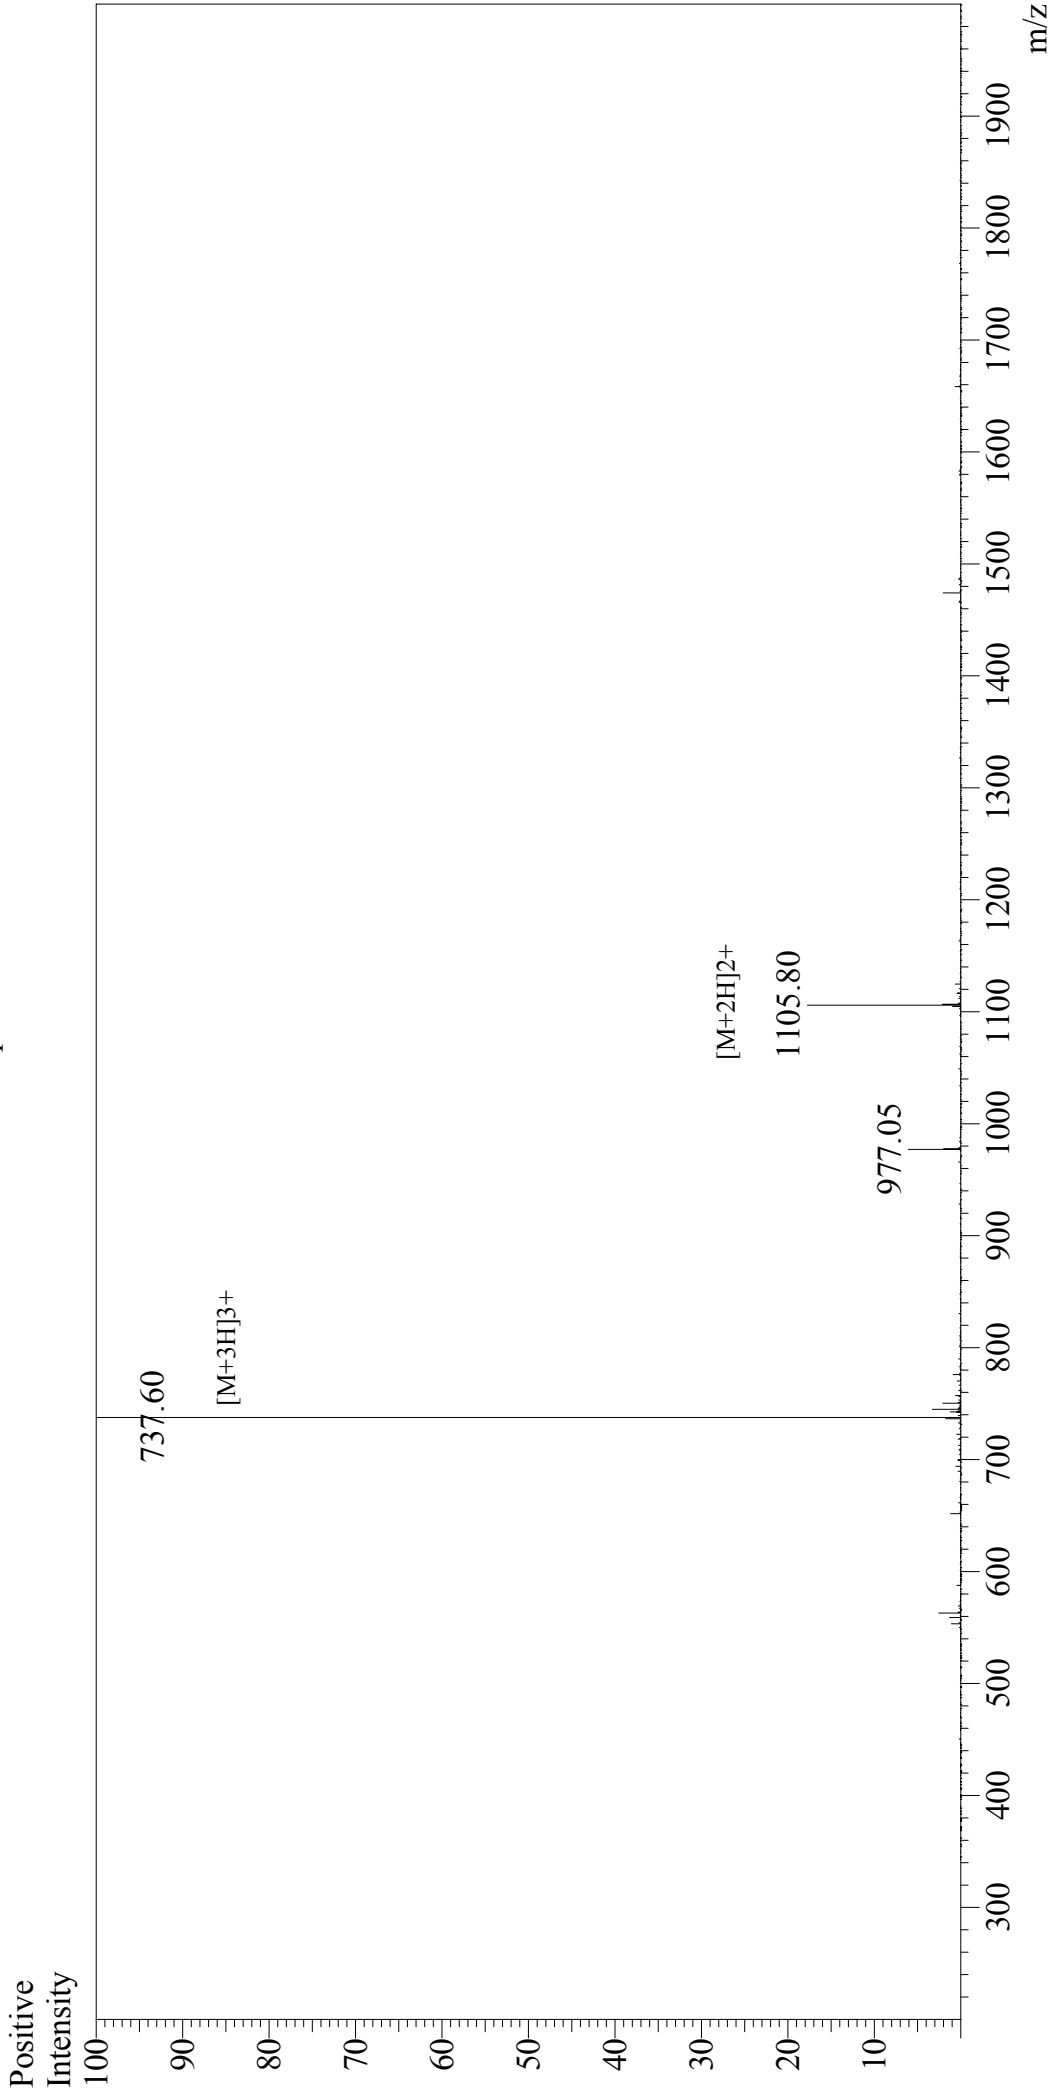

Sample Information

User : Gary
Month-Day Processed : 06/26/18
Time Processed : 13:31:41
Injection Volume : 0.2
Sample Name : HPV E7 protein (49-57)
Cat No. : RP11841
Lot No. : PE2721806
Theoretical MW : 2209.51
Observed MW : 2209.80

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias

Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH