


Mass Spectrum

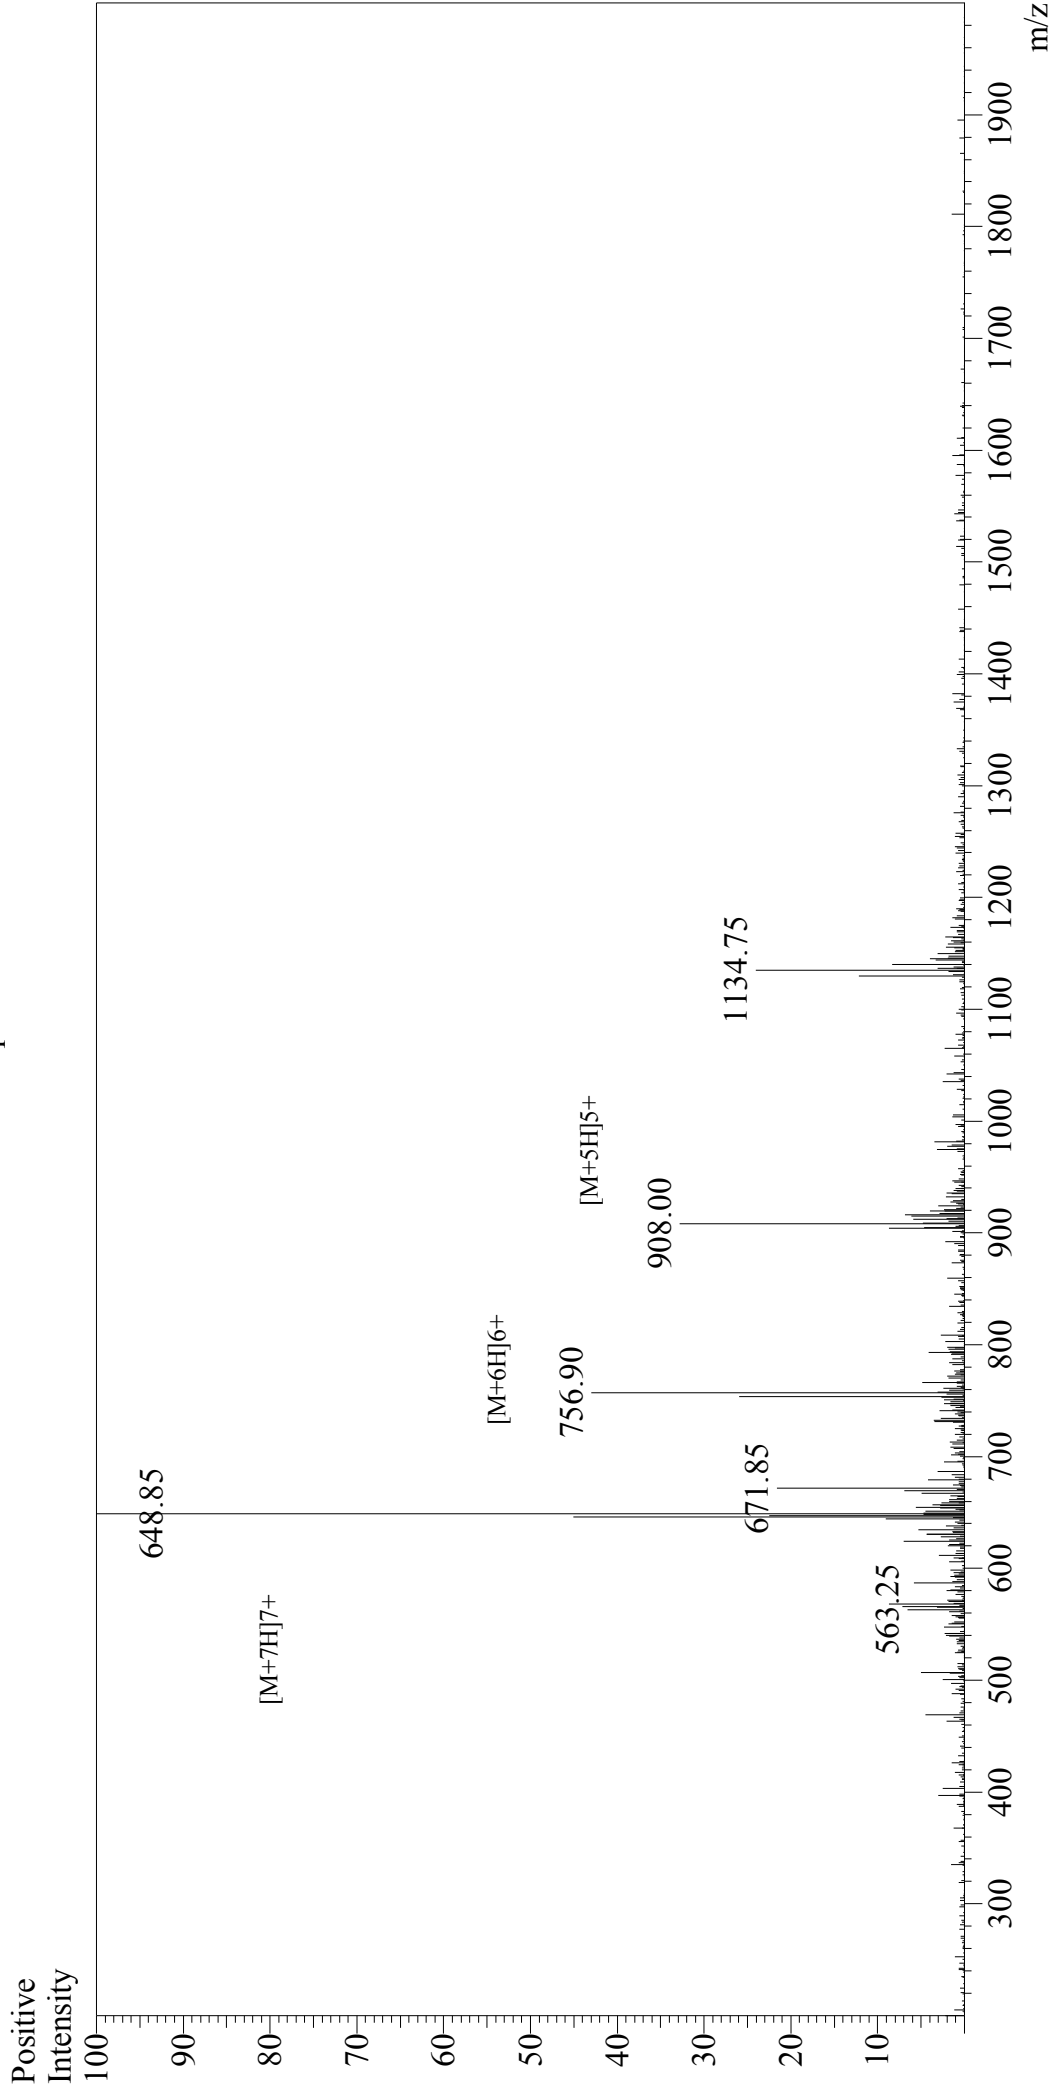

Sample Information

User : Gary
Month-Day Processed : 03/06/18
Time Processed : 17:37:49
Injection Volume : 0.2
Sample Name : PACAP(1-38),human,ovine,rat
Cat No. : RPI0335
Lot No. : PE2981803
Theoretical MW : 4534.26
Observed MW : 4534.95

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH