

Sample Name :N-Boc-Phe-Leu-Phe-Leu-Phe  
 Sample ID :U2530DJ250-1  
 Time Processed :17:00:49  
 Month-Day-Year Processed :11/08/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	40
25.00	Pumps	Pump A B.Conc	100
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	40
40.00	Pumps	Pump A B.Conc	40
45.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm  
 Equipment:ZJ17010508

<Chromatogram>

mV

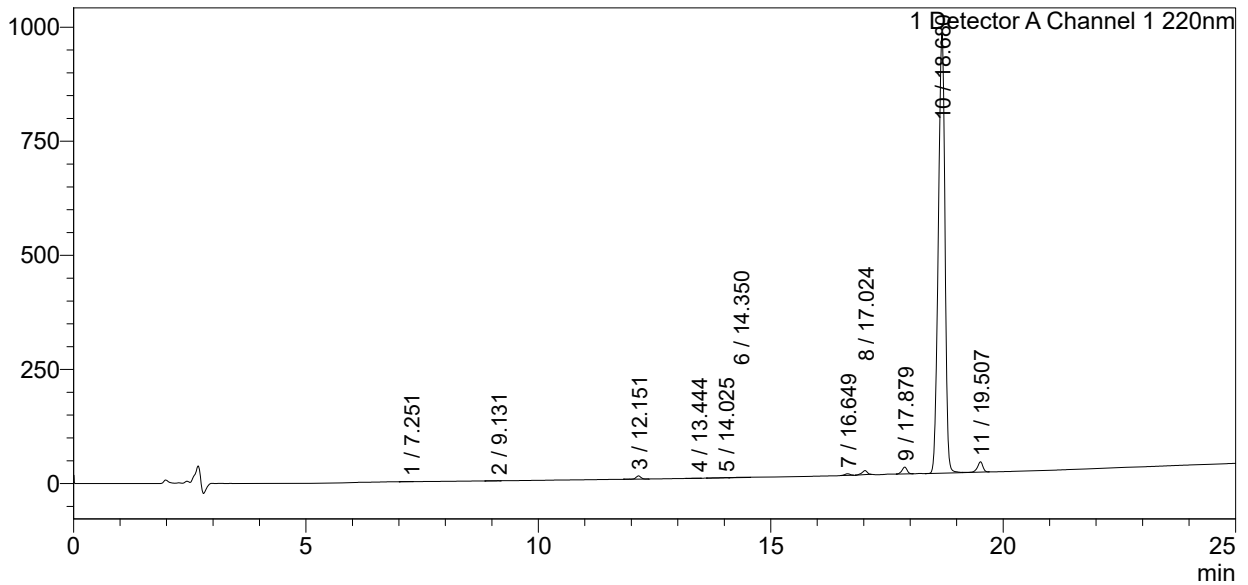

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.251	1545	150	0.015
2	9.131	1480	81	0.015
3	12.151	52968	7148	0.528
4	13.444	1419	124	0.014
5	14.025	4204	326	0.042
6	14.350	11117	772	0.111
7	16.649	25949	3464	0.259
8	17.024	69079	8772	0.689
9	17.879	113637	15009	1.134
10	18.680	9557677	963305	95.339
11	19.507	185840	22641	1.854
Total		10024914	1021791	100.000