

Sample Name: Angiotensin II (1-4), human
 Cat No. :RP11252
 Lot No. :E6253720I
 Time Processed: 9:03:25 AM
 Month-Day-Year Processed :09/14/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

mV

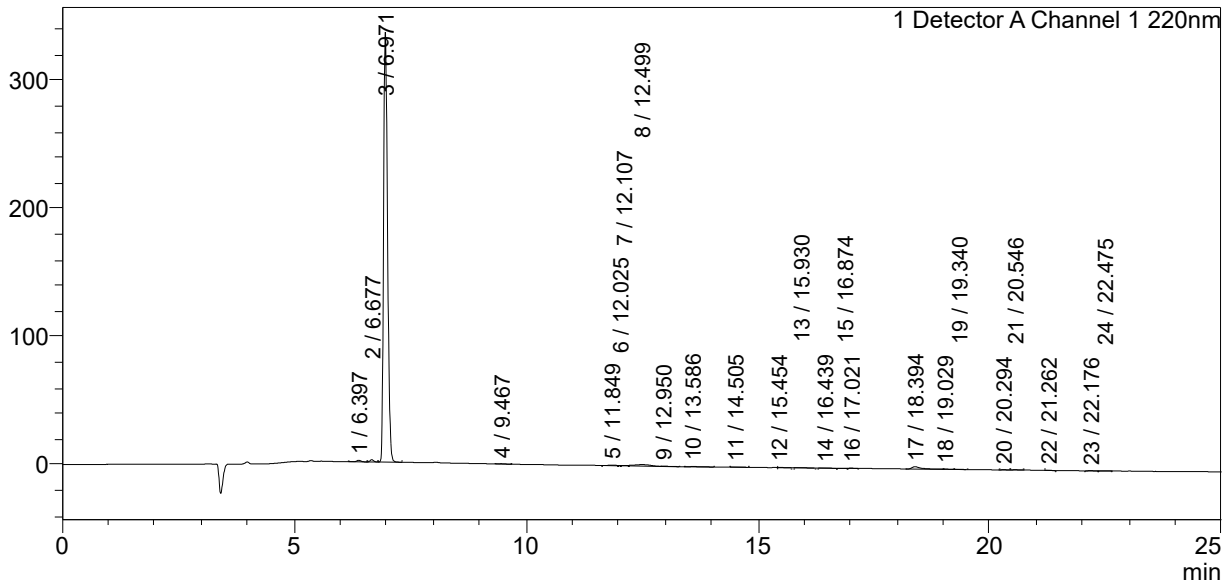

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.397	6950	1215	0.328
2	6.677	9409	1791	0.445
3	6.971	2011502	335984	95.069
4	9.467	1657	227	0.078
5	11.849	3031	190	0.143
6	12.025	1161	264	0.055
7	12.107	2391	321	0.113
8	12.499	26987	1087	1.275
9	12.950	1585	59	0.075
10	13.586	3825	159	0.181
11	14.505	1003	55	0.047
12	15.454	1711	140	0.081
13	15.930	1692	112	0.080
14	16.439	1342	98	0.063

Peak#	Ret. Time	Area	Height	Area%
15	16.874	1009	118	0.048
16	17.021	1673	251	0.079
17	18.394	29286	1889	1.384
18	19.029	2298	272	0.109
19	19.340	1246	137	0.059
20	20.294	1062	164	0.050
21	20.546	1535	165	0.073
22	21.262	1238	164	0.059
23	22.176	1230	188	0.058
24	22.475	1021	110	0.048
Total		2115844	345161	100.000