

Sample Name : LL37 (Human)  
 Cat. No. : RP13323  
 Lot. No. : E4880919I  
 Time Processed :15:41:05  
 Month-Day-Year Processed :09/12/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
95.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

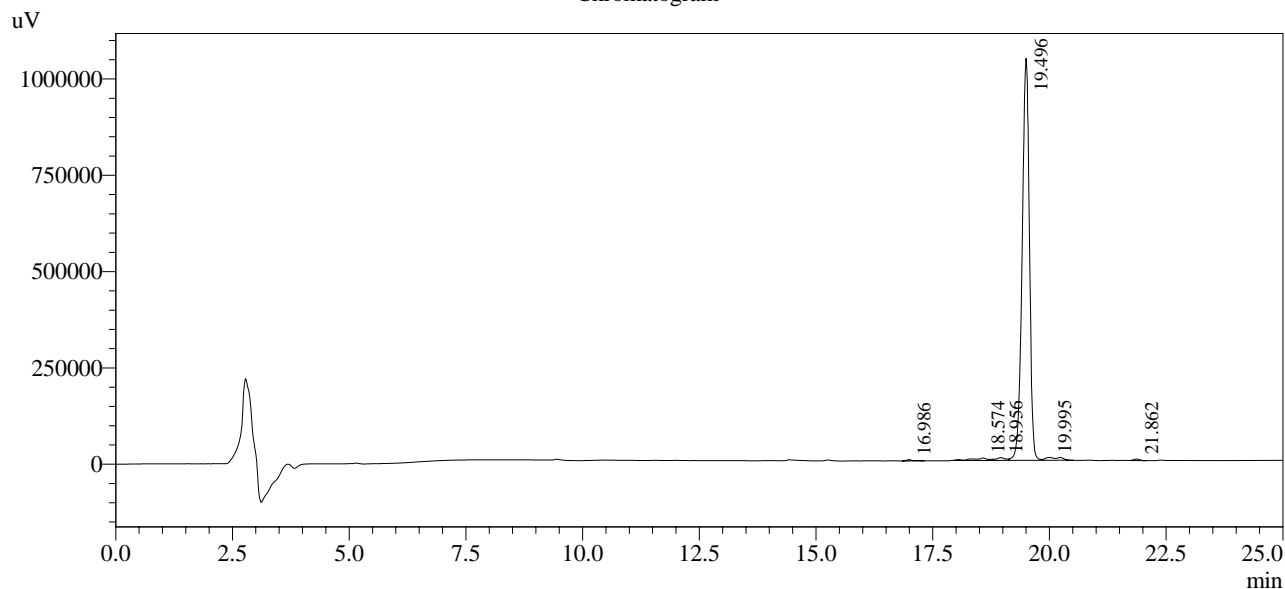

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.986	23544	3088	0.200
2	18.574	155214	6247	1.320
3	18.956	95324	7165	0.811
4	19.496	11278317	1043775	95.943
5	19.995	167047	7568	1.421
6	21.862	35778	4028	0.304
Total		11755224	1071871	100.000