

Sample Name : Influenza HA (518-526)
 Cat. No. : RP20284
 Lot. No. : PE2081612

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

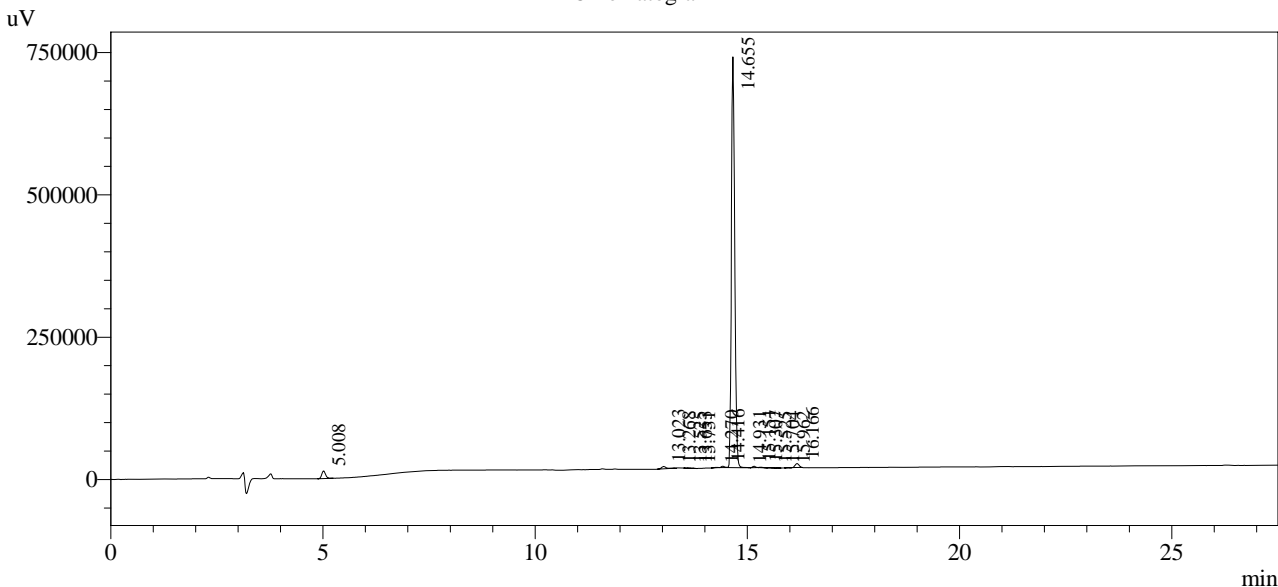

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.008	83905	13360	2.013
2	13.023	29330	4135	0.704
3	13.268	3300	294	0.079
4	13.525	162	107	0.004
5	13.653	1300	302	0.031
6	13.731	623	185	0.015
7	14.270	4242	694	0.102
8	14.416	12508	2334	0.300
9	14.655	3966255	721566	95.149
10	14.931	3189	588	0.076
11	15.151	11238	2333	0.270
12	15.307	4010	655	0.096
13	15.525	1690	327	0.041
14	15.704	617	222	0.015
15	15.962	1873	426	0.045
16	16.166	44213	6846	1.061
Total		4168455	754372	100.000