

Sample Name :VIP, human, ovine, porcine, rat

Cat No.: RP10085

Lot No.: E4017320H

Time Processed: 10:14:22 AM

Month-Day-Year Processed :9/11/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.00	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment:ZJ19010325

<Chromatogram>

mV

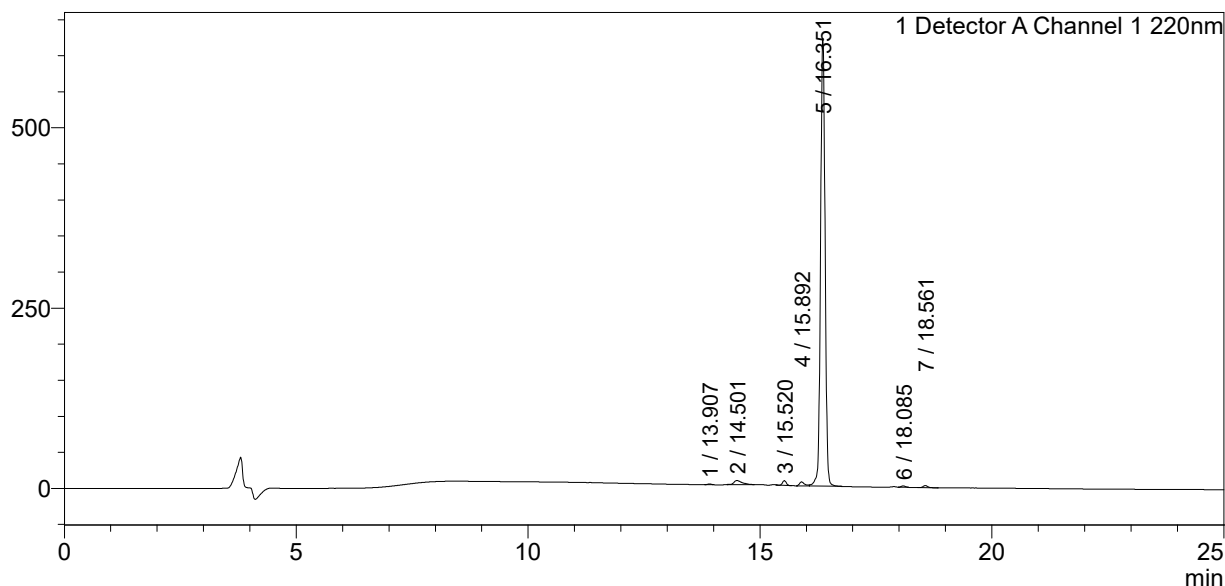

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.907	5090	1015	0.116
2	14.501	67258	5530	1.534
3	15.520	34804	6503	0.794
4	15.892	42957	5483	0.980
5	16.351	4205703	621109	95.901
6	18.085	10771	1851	0.246
7	18.561	18885	2918	0.431
Total		4385468	644409	100.000