

Sample Name :LSKL, Inhibitor of Thrombospondin (TSP-1)

Cat No: RP19990

Lot No: PE9371803

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

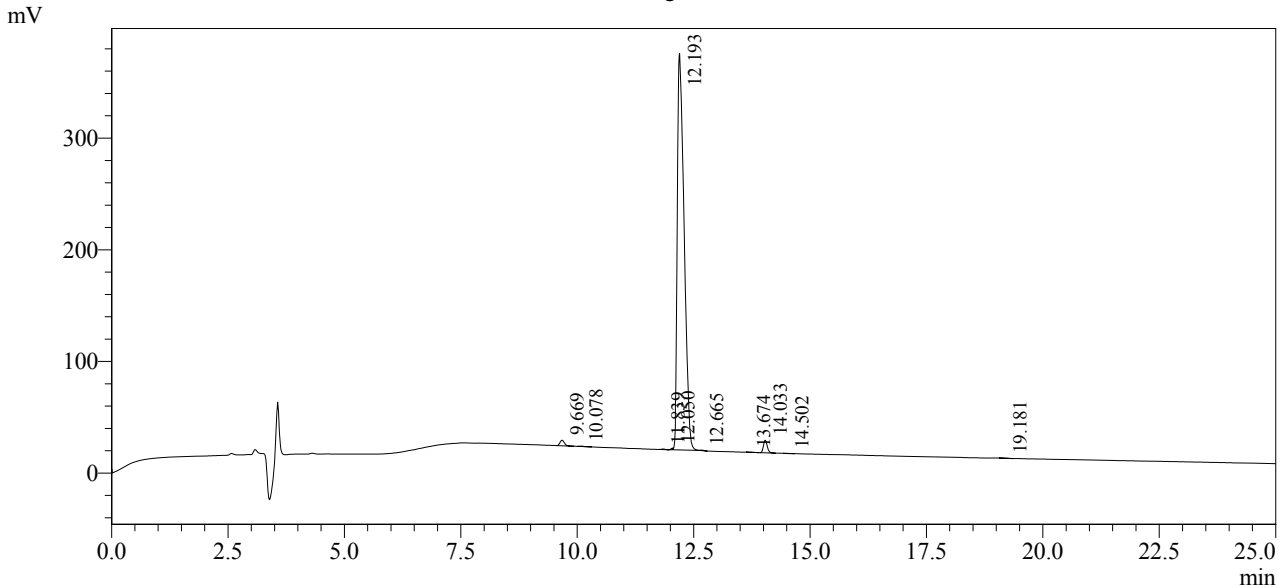

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.669	33219	5017	0.886
2	10.078	2368	386	0.063
3	11.839	2787	552	0.074
4	12.050	4852	1584	0.129
5	12.193	3633734	355240	96.934
6	12.665	2318	500	0.062
7	13.674	1262	123	0.034
8	14.033	64357	11291	1.717
9	14.502	2028	360	0.054
10	19.181	1730	212	0.046
Total		3748656	375267	100.000