

Sample Name : Ghrelin, rat  
 Cat No. : RP10781  
 Lot No. : E5449121A  
 Time Processed : 20:20:09  
 Month-Day-Year Processed : 01/20/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
45.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

mV

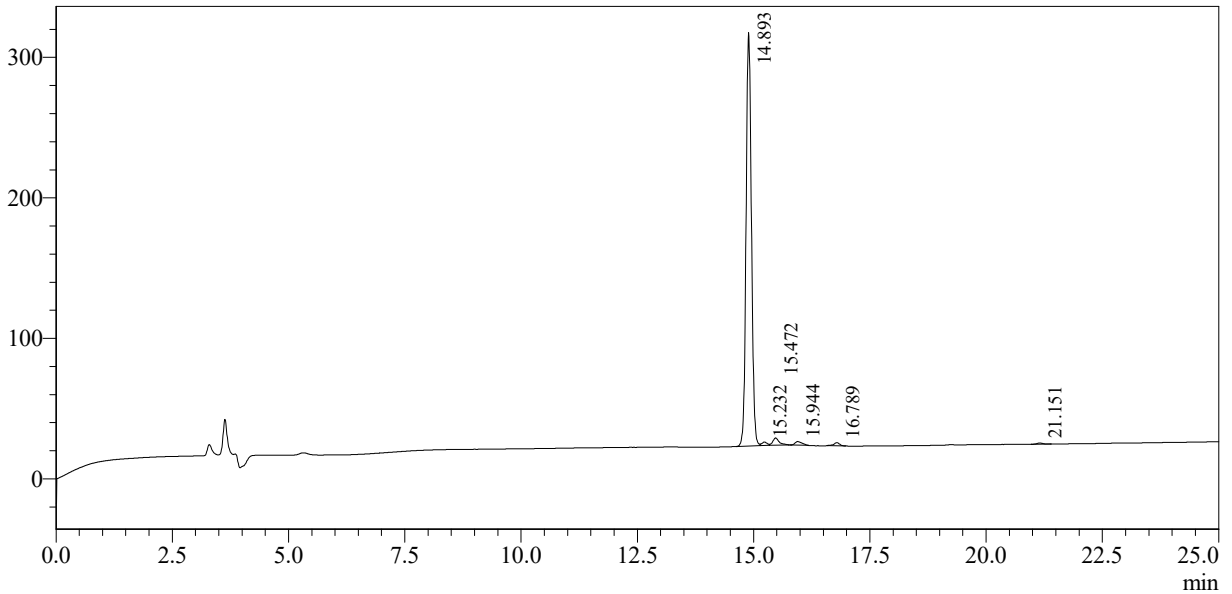

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.893	2354789	294223	95.144
2	15.232	20080	2533	0.811
3	15.472	47896	5072	1.935
4	15.944	26426	2519	1.068
5	16.789	18972	2213	0.767
6	21.151	6804	808	0.275
Total		2474967	307368	100.000