

Sample Name : VIP, human, ovine, porcine, rat
 Cat. No. : RP10085
 Lot. No. : PE3631803

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

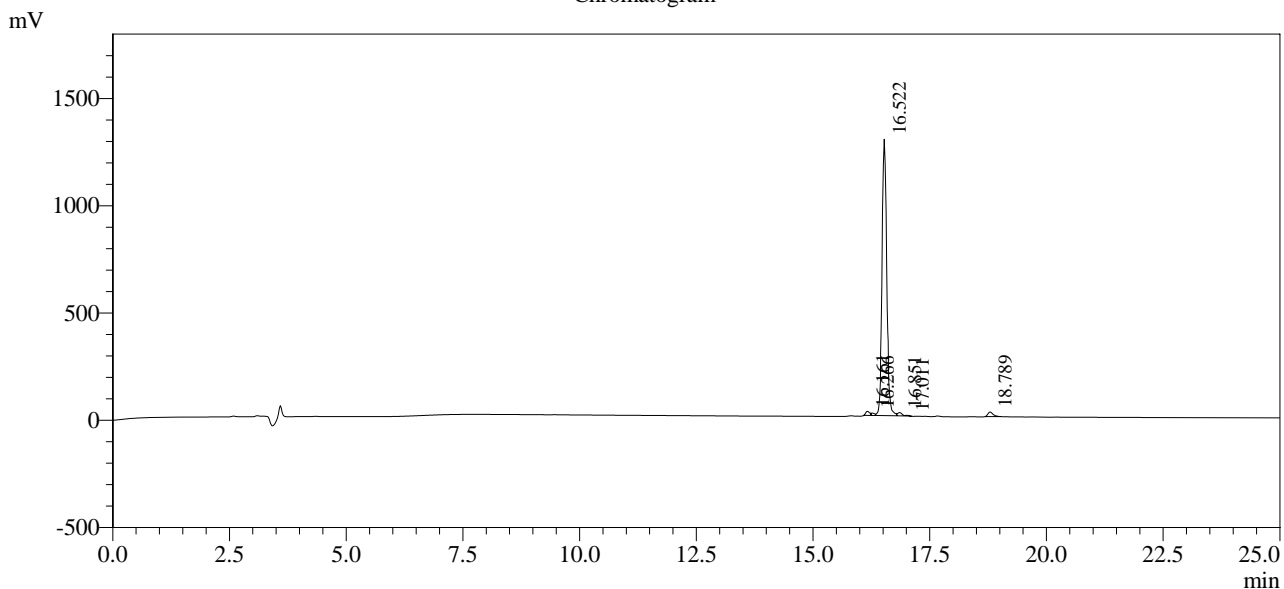

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.161	112953	18728	1.183
2	16.266	54224	10792	0.568
3	16.522	9106225	1288074	95.346
4	16.851	101285	15586	1.061
5	17.011	18777	3673	0.197
6	18.789	157212	21062	1.646
Total		9550676	1357915	100.000