


# Mass Spectrum

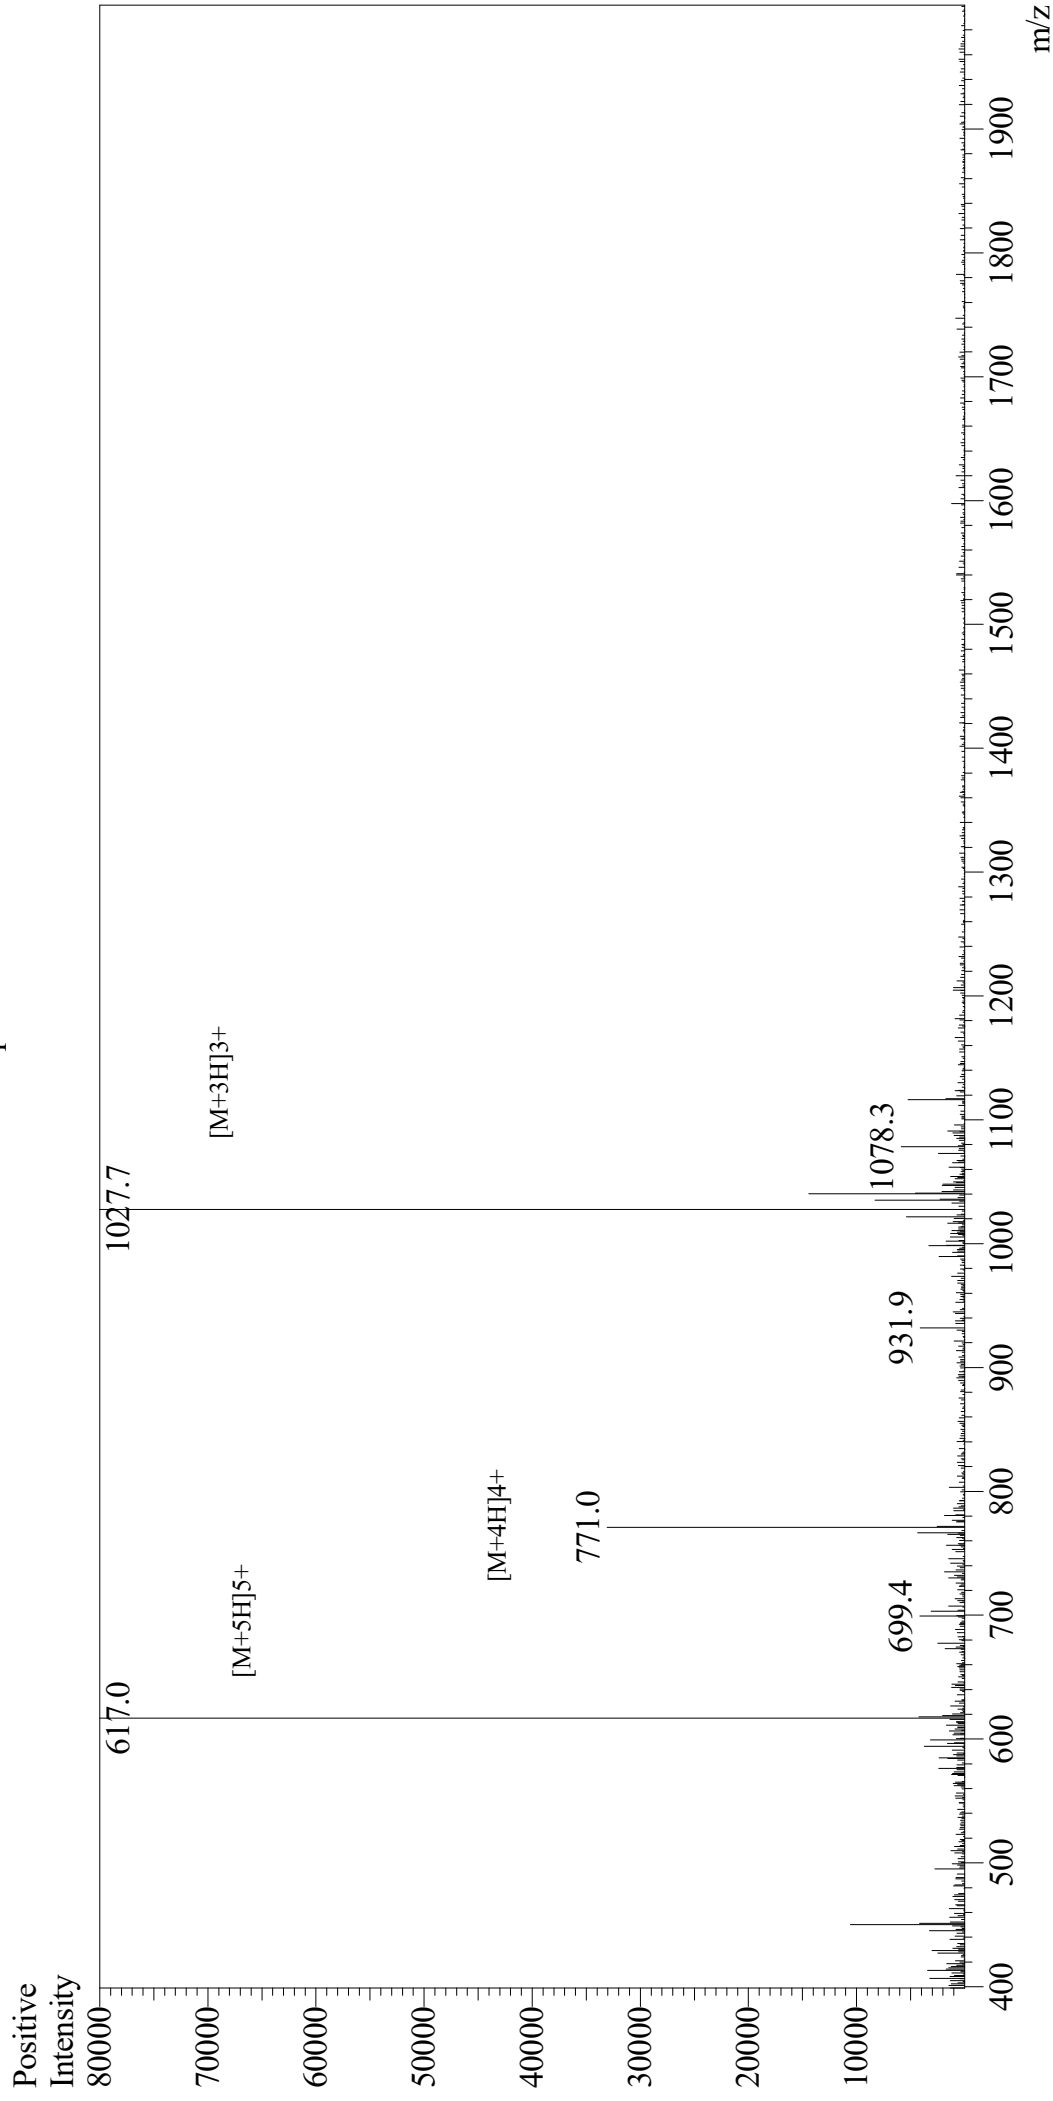

<b>Sample Information</b>	<b>Interface</b> : ESI	<b>Interface Bias</b> : +4.5kV
User : Gary	<b>Nebulizing Gas Flow</b> : 1.5L/min	<b>Drying Gas Flow</b> : 5 L/min
Month-Day Processed : 08/23/18	<b>CDL Temp</b> : 250 $\pm$ æ	<b>T.Flow</b> : 0.2ml/min
Time Processed : 2:02:22 PM	<b>Block Temp</b> : 200 $\pm$ æ	<b>B.conc</b> : 50% $\text{H}_2\text{O}/50\%\text{MeOH}$
Injection Volume : 0.8		
Sample Name : ANP (1-28), human, porcine		
Cat No. : RP11927		
Lot No. : PE5401808		
Theoretical MW : 3080.50		
Observed MW : 3080.1		