

Sample Name :ACTH) (1-24), human
 Cat No. :RP11303
 Lot No. :PE0261811
 Time Processed :9:10:16
 Month-Day-Year Processed :11/06/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

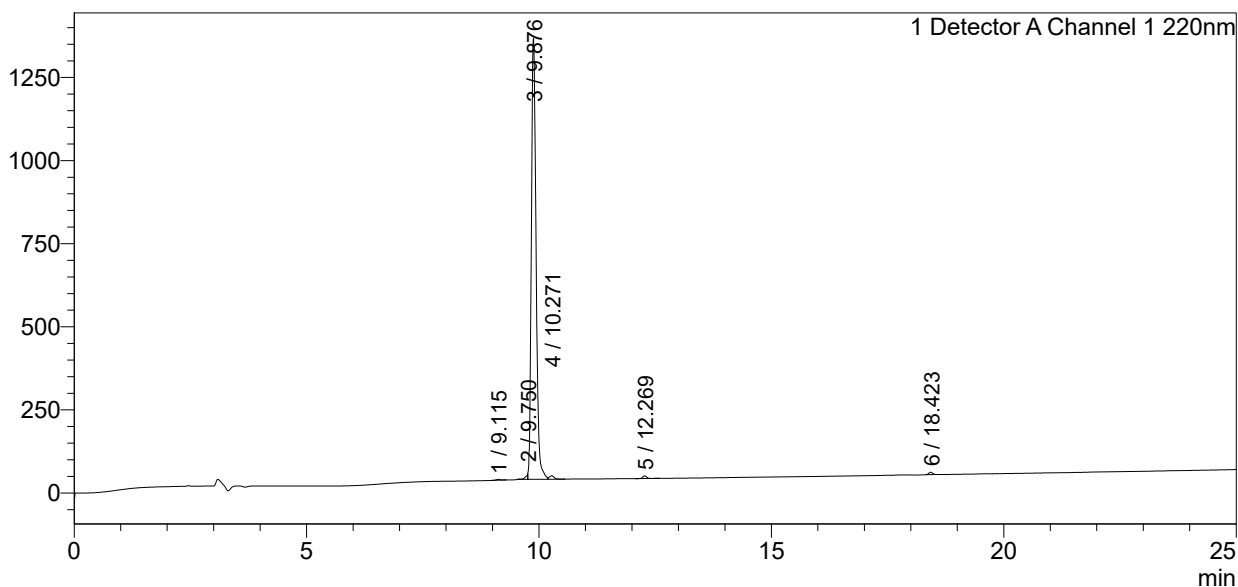

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.115	15966	2577	0.167
2	9.750	56402	13138	0.591
3	9.876	9321449	1325950	97.609
4	10.271	73065	10472	0.765
5	12.269	43946	7944	0.460
6	18.423	39006	6910	0.408
Total		9549833	1366991	100.000