

Sample Name :Speract
 Cat No. : RP10620
 Lot No. : E5564619J
 Time Processed : 23:05:09
 Month-Day-Year Processed : 10/10/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

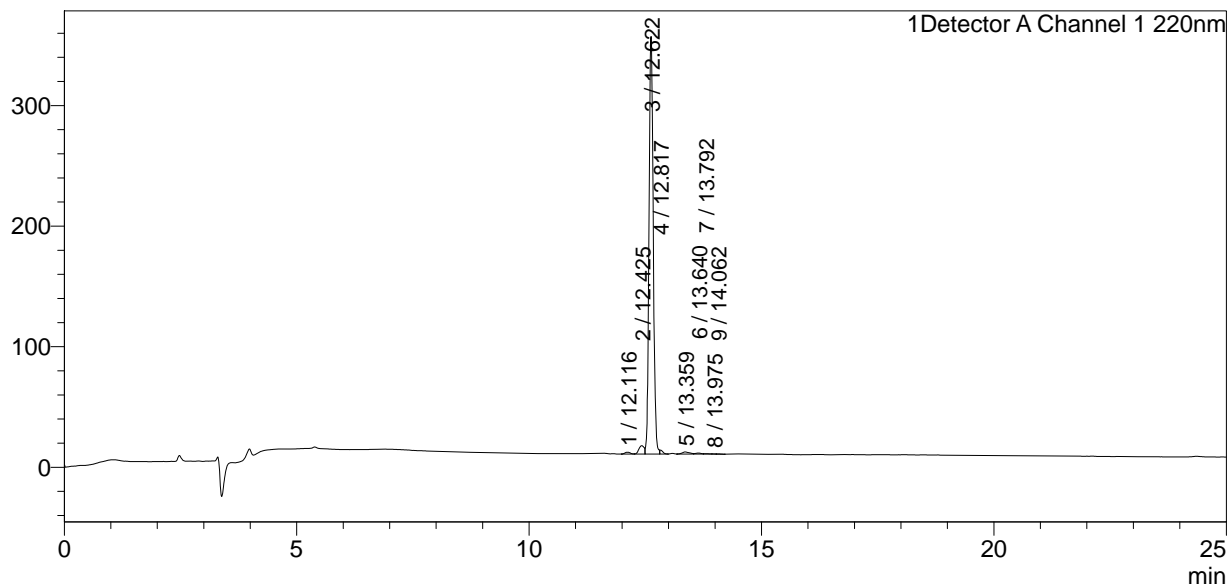

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.116	12104	1516	0.527
2	12.425	55042	6898	2.397
3	12.622	2184349	346270	95.115
4	12.817	13853	3250	0.603
5	13.359	18739	1707	0.816
6	13.640	7349	877	0.320
7	13.792	2973	351	0.129
8	13.975	999	203	0.043
9	14.062	1129	181	0.049
Total		2296536	361253	100.000