

Sample Name : BDC2.5 mimotope 1040-31  
 Cat. No. : RP20518  
 Lot. No. : E7113819J  
 Time Processed :14:01:05  
 Month-Day-Year Processed :10/08/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	20	
25.00	Pumps	Pump A B.Conc	80	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

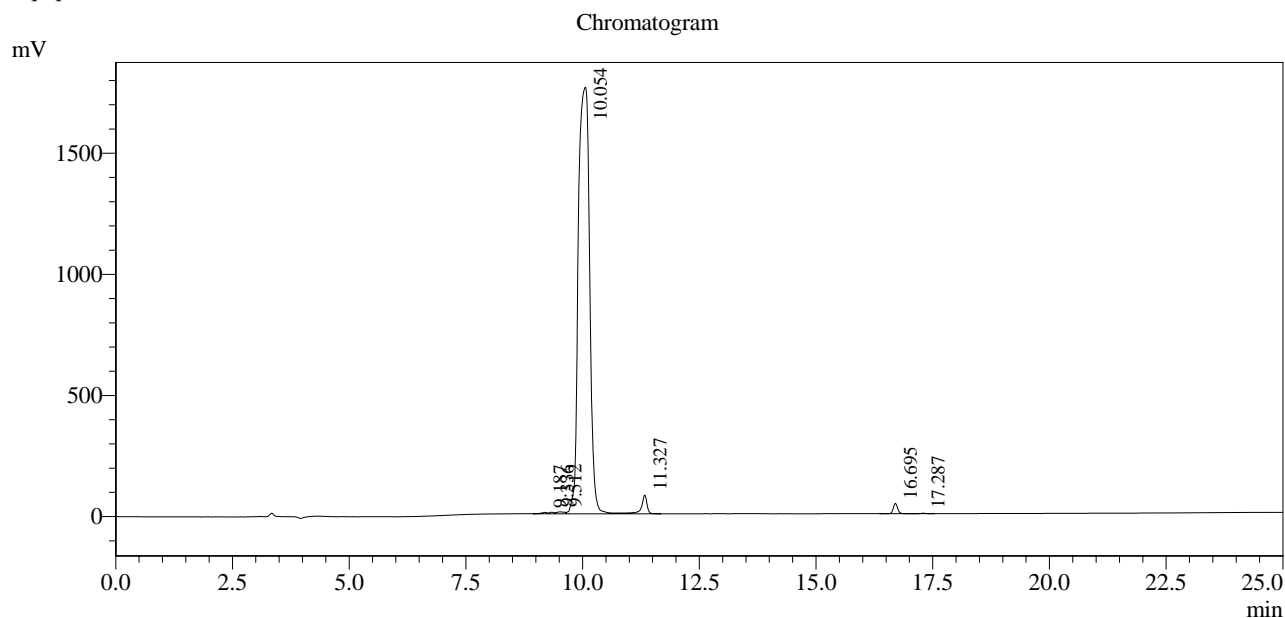

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.187	51193	5712	0.167
2	9.336	44287	6734	0.144
3	9.512	93324	8036	0.304
4	10.054	29580945	1760910	96.291
5	11.327	662868	77177	2.158
6	16.695	275710	42358	0.897
7	17.287	12003	1780	0.039
Total		30720331	1902706	100.000