

Sample Name : Myomodulin
 Cat.No : RP10606
 Lot.No : E5808920C
 Time Processed: 11:53:56
 Year-Month-Day: 2020/3/30

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
33.00	Pumps	Solvent B Conc.	5	
33.01	Controller	Stop		

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010015

<Chromatogram>

mV

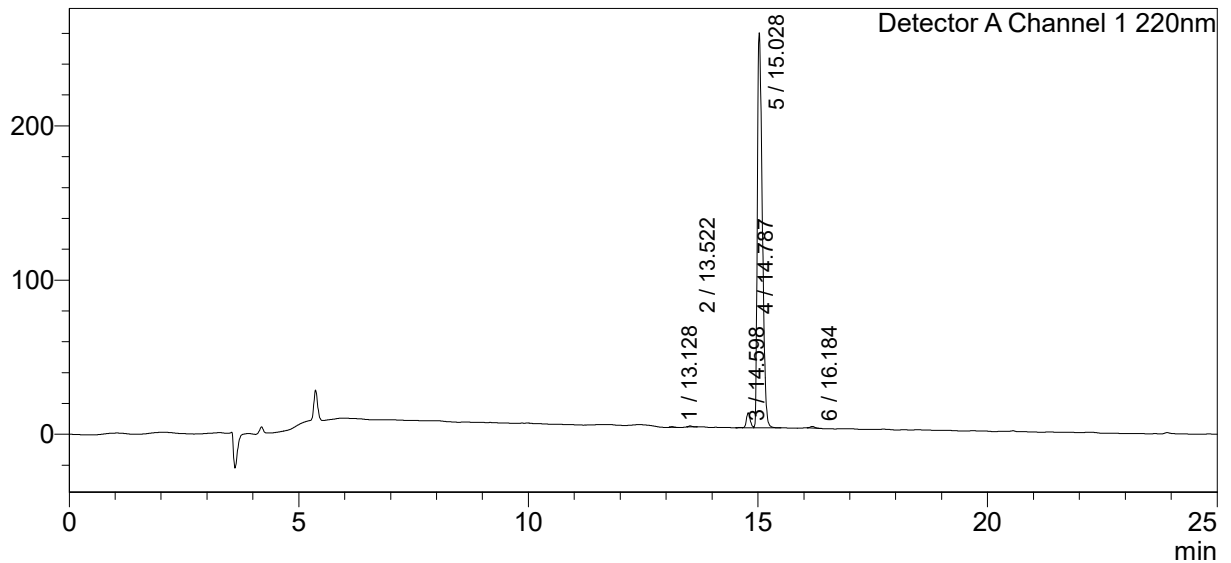

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.128	2487	460	0.124
2	13.522	3285	591	0.164
3	14.598	1608	282	0.080
4	14.787	57048	9893	2.841
5	15.028	1936240	256192	96.440
6	16.184	7039	1022	0.351
Total		2007706	268439	100.000