

Sample Name :C3a (70-77)
 Cat No. :RP20511
 Lot No. :PE9031902
 Time Processed : 9:29:55
 Month-Day-Year Processed : 03/05/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

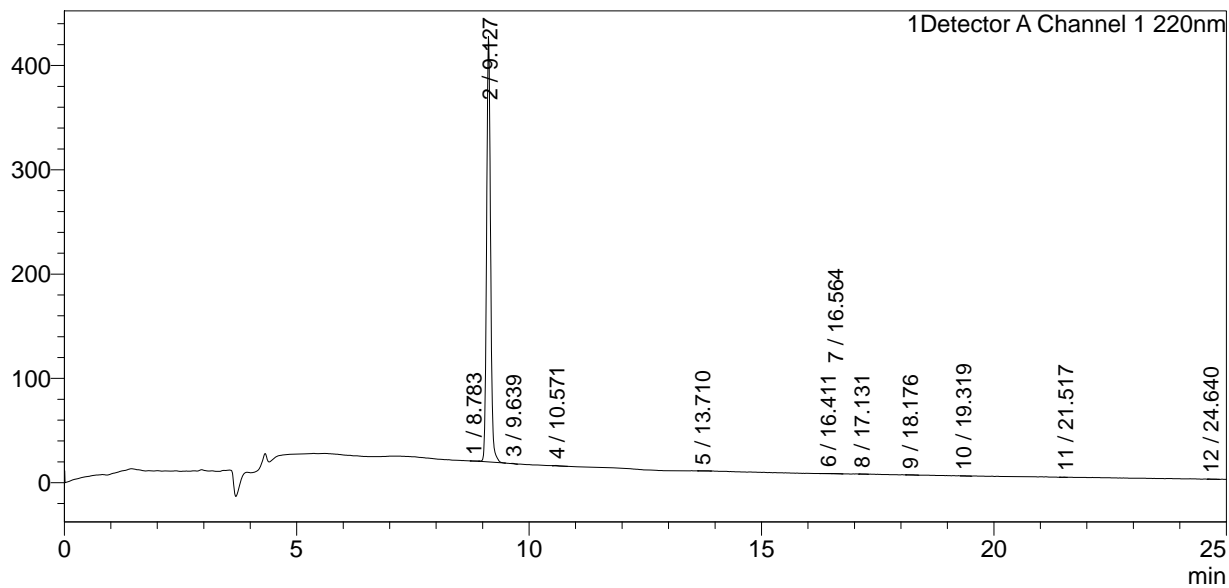

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.783	1143	196	0.047
2	9.127	2408546	407851	99.294
3	9.639	1031	251	0.043
4	10.571	2863	399	0.118
5	13.710	1590	135	0.066
6	16.411	2495	240	0.103
7	16.564	1624	185	0.067
8	17.131	1175	159	0.048
9	18.176	1449	156	0.060
10	19.319	1356	178	0.056
11	21.517	1083	188	0.045
12	24.640	1313	158	0.054
Total		2425668	410097	100.000