

Sample Name : PLP(139-151)  
 Cat. No. : RP10550  
 Lot. No. : PE2751805

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

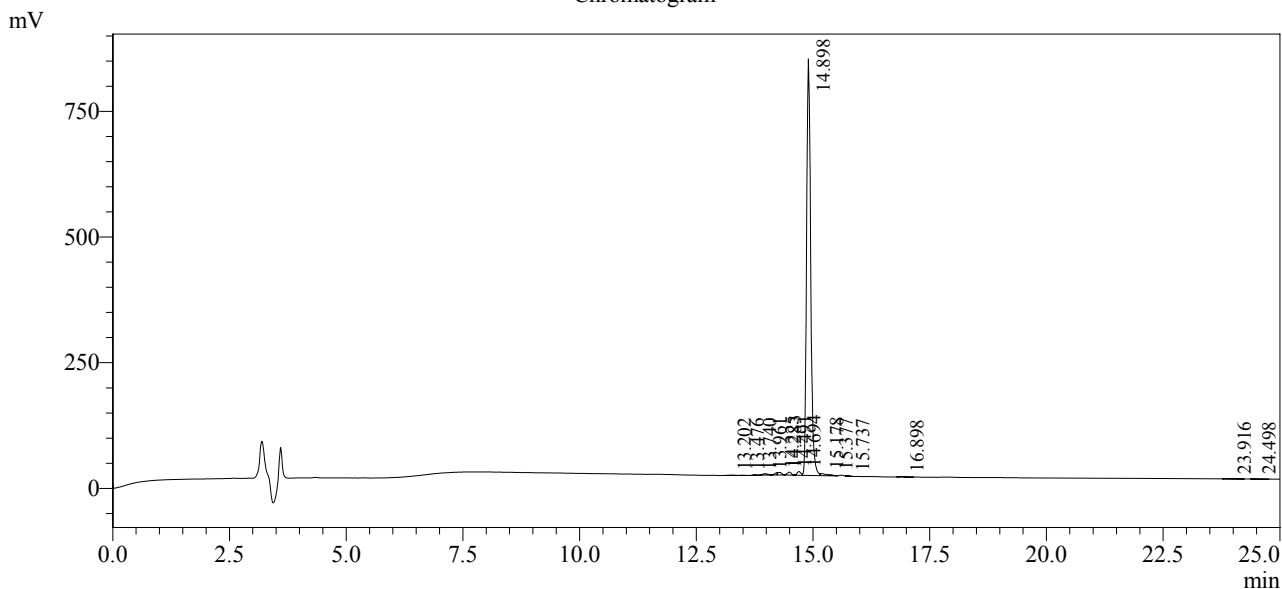

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.202	6361	608	0.120
2	13.476	3683	668	0.069
3	13.740	5991	1205	0.113
4	13.961	21254	2752	0.400
5	14.225	17817	4490	0.335
6	14.283	30637	5258	0.577
7	14.491	35142	5816	0.661
8	14.694	41919	7399	0.789
9	14.898	5089152	828565	95.788
10	15.178	35785	3958	0.674
11	15.377	9195	2032	0.173
12	15.737	2261	543	0.043
13	16.898	4753	727	0.089
14	23.916	4855	569	0.091
15	24.498	4148	421	0.078
Total		5312950	865010	100.000