

Sample Name :Calcitonin, salmon
Cat. No. : RP11099
Lot. No. : PE2871809
Time Processed : 8:15:57
Month-Day-Year Processed : 10/11/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
30.00	Pumps	Pump A B.Conc	95	
30.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

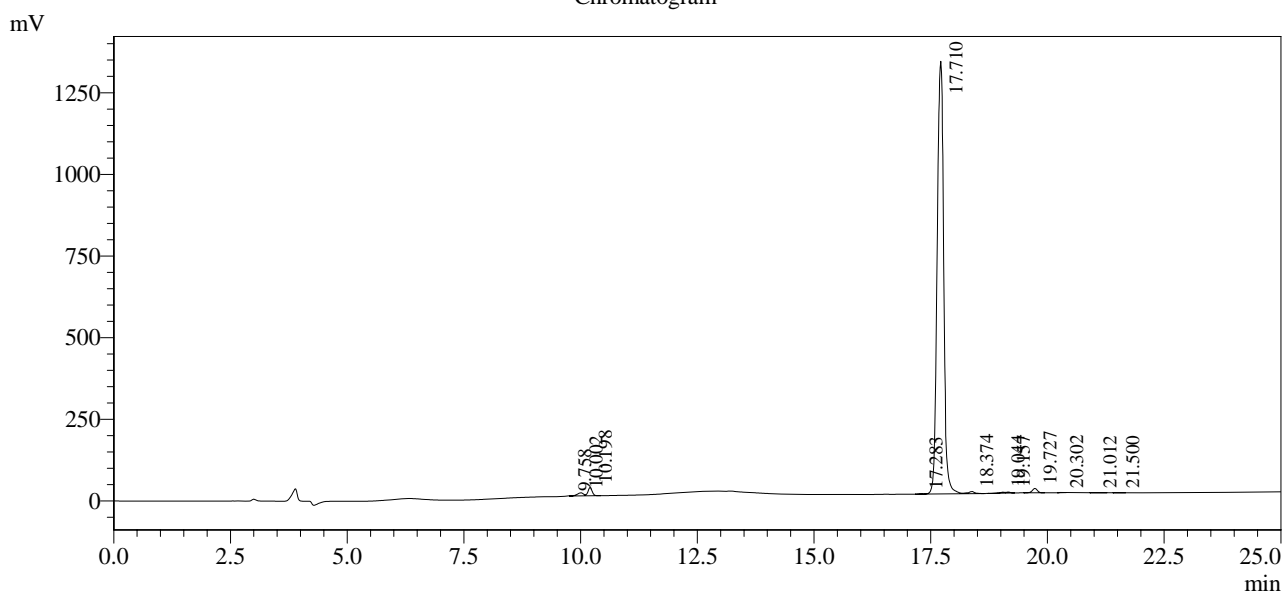

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.758	-168	0	-0.001
2	10.002	88325	9574	0.662
3	10.198	157897	25312	1.183
4	17.283	4917	739	0.037
5	17.710	12874554	1324954	96.476
6	18.374	65146	6784	0.488
7	19.044	25076	2965	0.188
8	19.157	18221	3056	0.137
9	19.727	100045	13226	0.750
10	20.302	4819	897	0.036
11	21.012	4492	584	0.034
12	21.500	1555	232	0.012
Total		13344879	1388324	100.000