

Sample Name :Moth Cytochrome C (MCC) (88-103)

Cat. No. : RP12808

Lot. No. : E1502620F

Time Processed: 2:36:22 AM

Month-Day-Year Processed :6/18/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment:ZJ19010325

### <Chromatogram>

mV

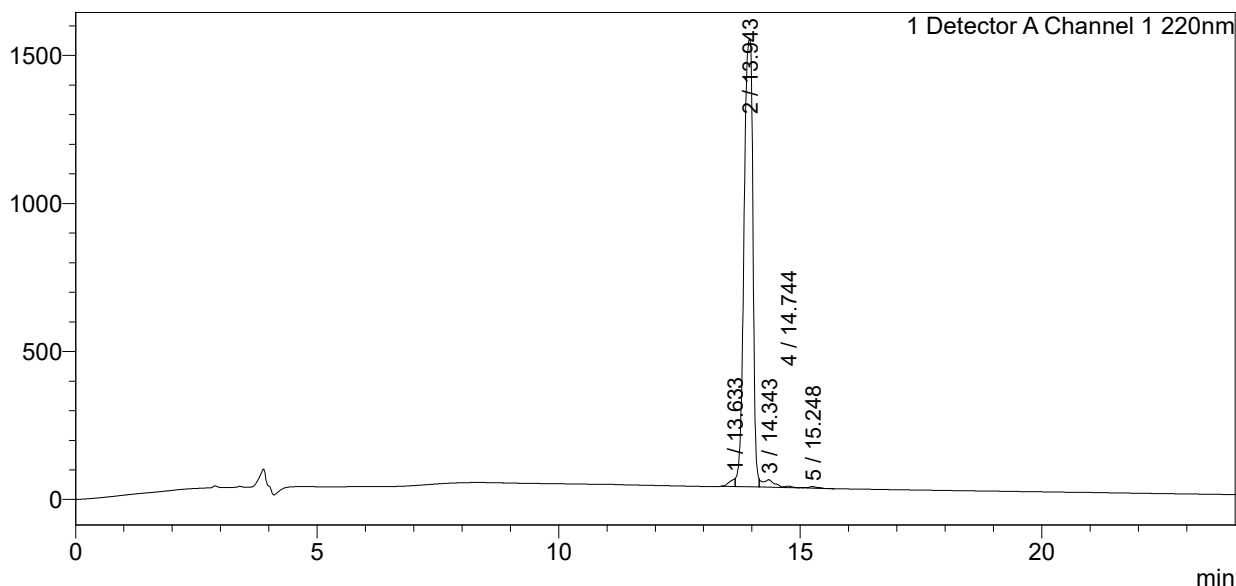

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.633	205407	24260	1.030
2	13.943	19139123	1505522	96.010
3	14.343	455335	25118	2.284
4	14.744	59636	5027	0.299
5	15.248	74970	5382	0.376
Total		19934470	1565309	100.000