

Sample Name :LAH4
 Cat. No. : RP20096
 Lot. No. : E8849220D
 Time Processed : 7:18:56
 Month-Day-Year Processed : 04/17/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

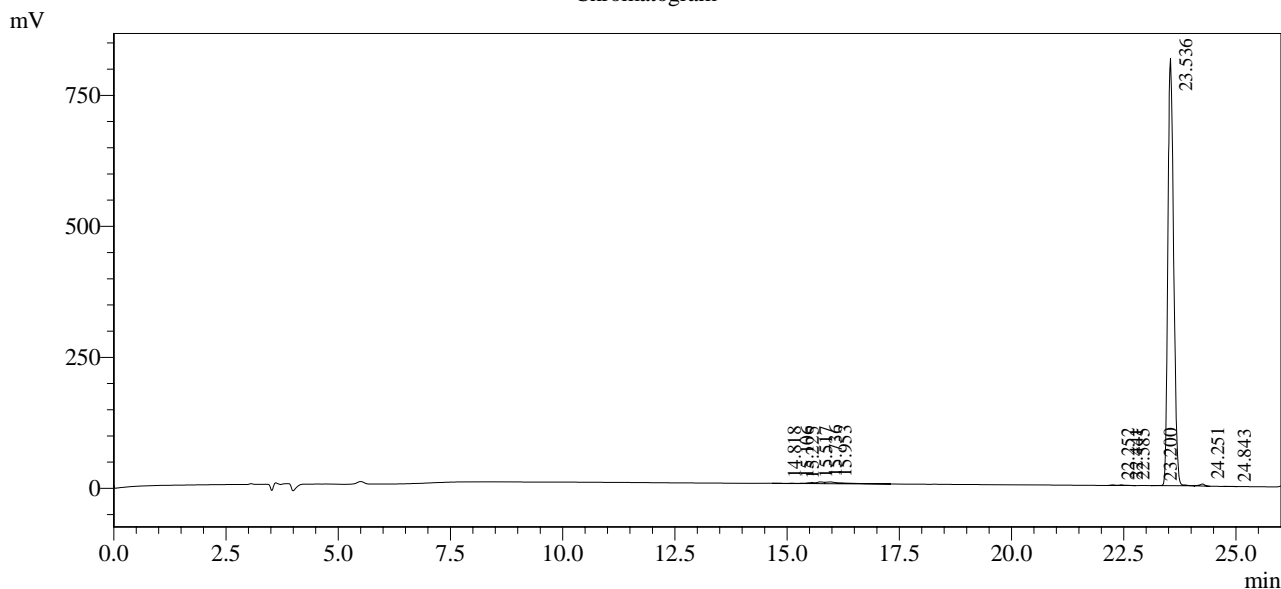

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.818	3903	405	0.052
2	15.106	5245	471	0.070
3	15.225	1526	388	0.020
4	15.517	17351	1563	0.231
5	15.736	40392	3430	0.537
6	15.953	95504	3334	1.270
7	22.252	7415	1024	0.099
8	22.441	7925	1195	0.105
9	22.585	2807	432	0.037
10	23.200	2933	411	0.039
11	23.536	7307270	815736	97.139
12	24.251	28535	3740	0.379
13	24.843	1681	219	0.022
Total		7522486	832348	100.000