

Sample Name :Prolactin Releasing Peptide (1-31), human
 Cat No. :RP11861
 Lot No. :E4875119I
 Time Processed :10:13:08 AM
 Month-Day-Year Processed :09/23/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
32.00	Pumps	Solvent B Conc.	95
32.01	Pumps	Solvent B Conc.	5
41.00	Pumps	Solvent B Conc.	5
45.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

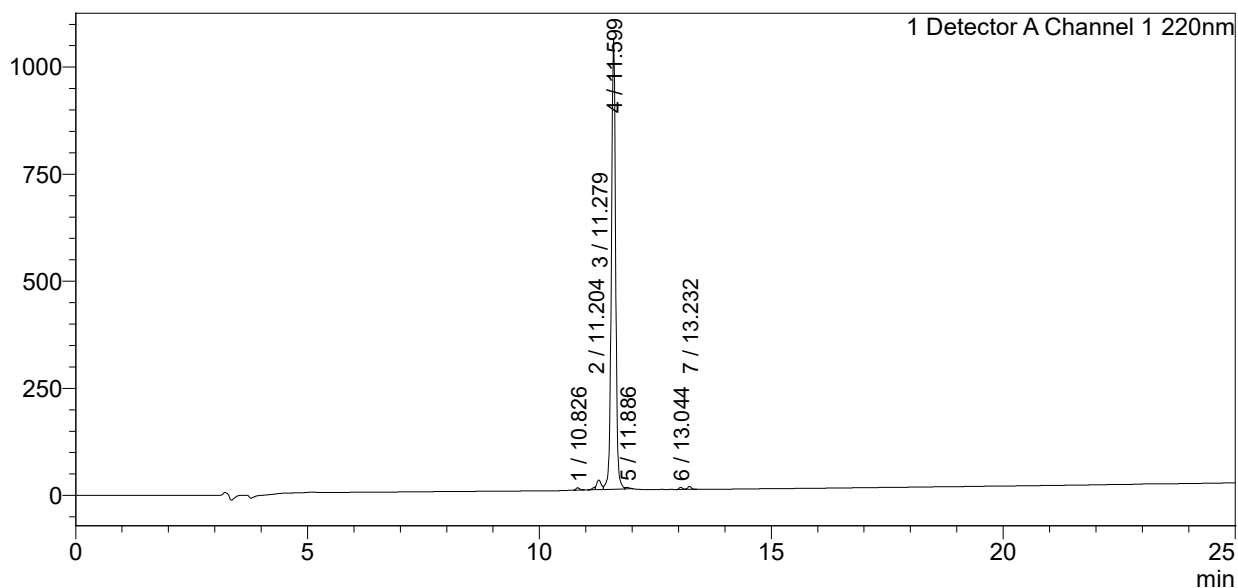

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.826	28243	5391	0.407
2	11.204	27695	6131	0.399
3	11.279	150534	22855	2.168
4	11.599	6656462	1051091	95.847
5	11.886	18501	3090	0.266
6	13.044	26534	5271	0.382
7	13.232	36878	6866	0.531
Total		6944848	1100694	100.000