


Mass Spectrum

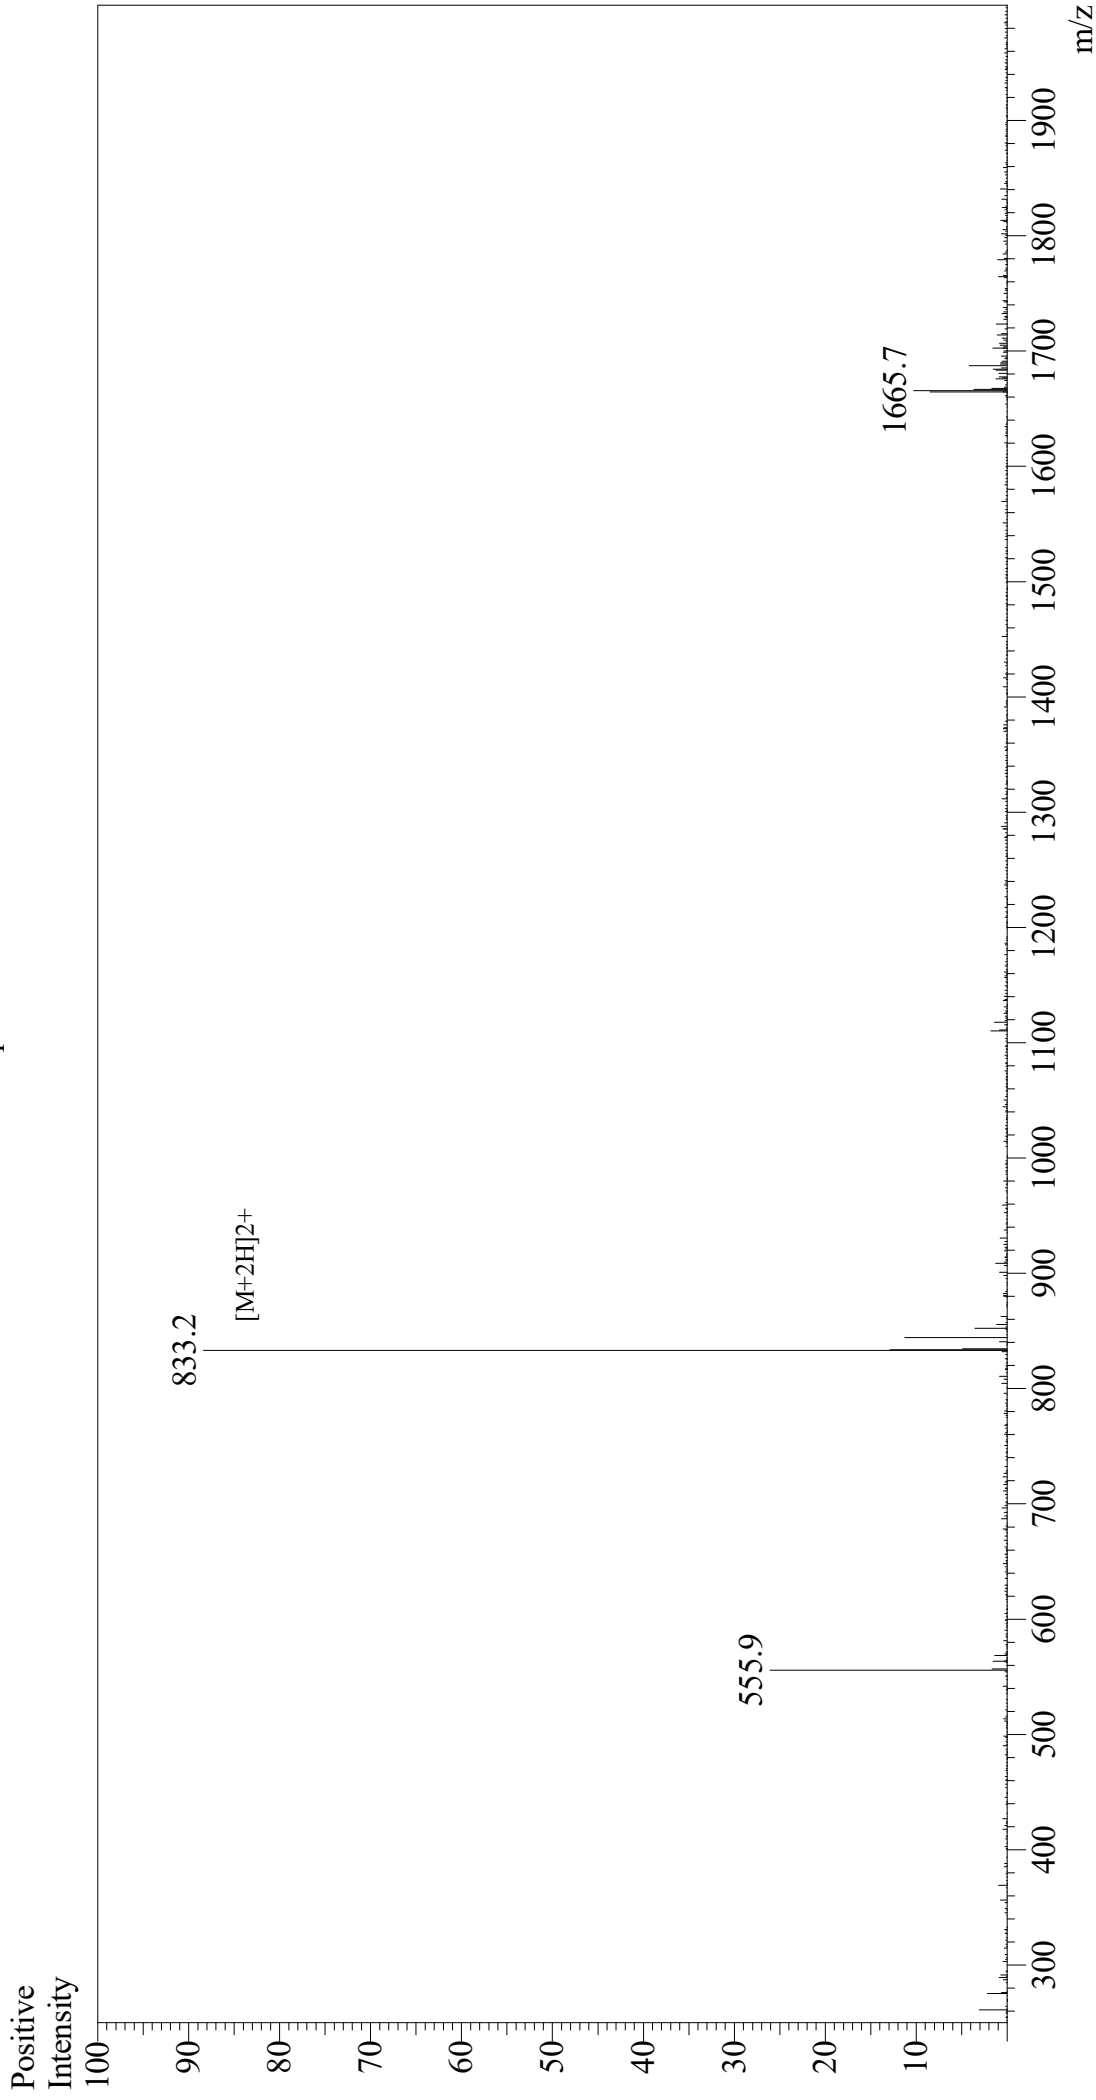

Sample Information

Month-Day Processed : 01/26/21
Time Processed : 7:18:30 PM
Injection Volume : 0.4
Sample Name : α -Melanocyte-Stimulating Hormone (MSH), amide
Cat No. : RP10644
Lot No. : E0669221A
Theoretical MW : 1664.90
Observed MW : 1664.4

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H₂O/50%MeOH