

Sample Name :[Sar1, Ile8]-Angiotensin II

Cat No. : RP13720 Lot No. : PE3321802

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

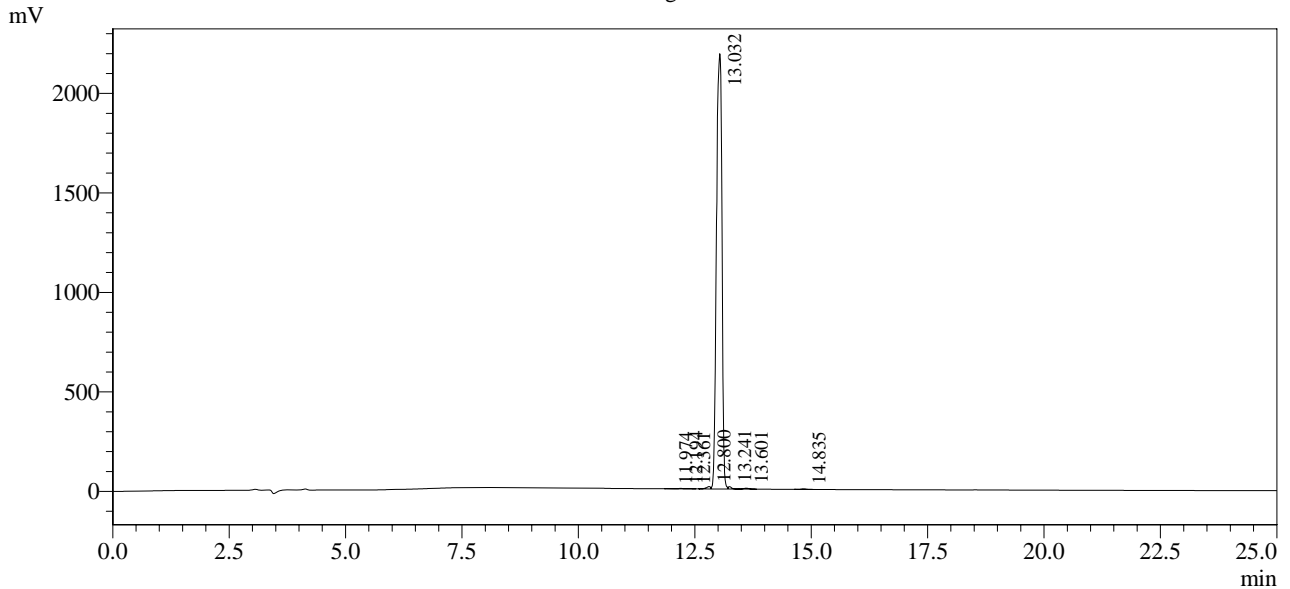

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.974	5261	723	0.029
2	12.194	16042	2454	0.089
3	12.361	9011	1220	0.050
4	12.800	76973	11867	0.425
5	13.032	17880576	2187359	98.773
6	13.241	57523	11664	0.318
7	13.601	35668	4311	0.197
8	14.835	21692	2710	0.120
Total		18102746	2222308	100.000