

Sample Name : GRGDSPC  
 Cat. No. : RP20283  
 Lot. No. : PE8331807

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

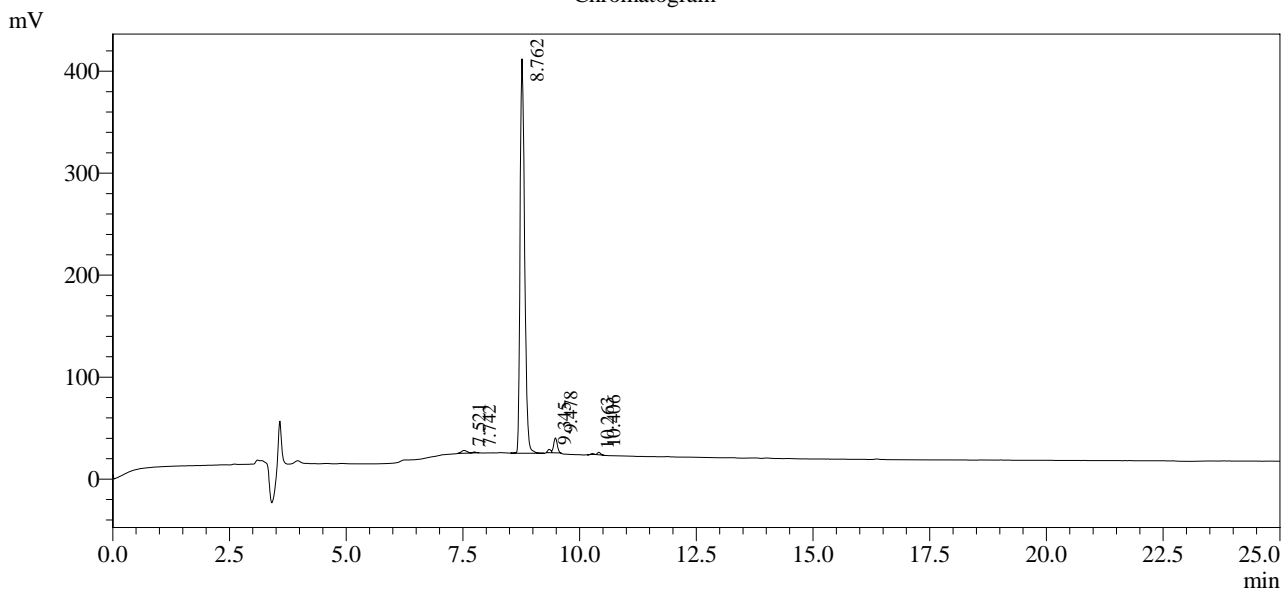

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.521	23941	2787	0.867
2	7.742	4702	893	0.170
3	8.762	2624798	386752	95.098
4	9.345	15420	3208	0.559
5	9.478	76924	14643	2.787
6	10.263	2617	743	0.095
7	10.406	11706	2440	0.424
Total		2760109	411466	100.000