

Sample Name :Crustacean Cardioactive Peptide (CCAP)
 Cat. No. : RP10572
 Lot. No. : PE4861812
 Time Processed : 9:40:08
 Month-Day-Year Processed : 01/13/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

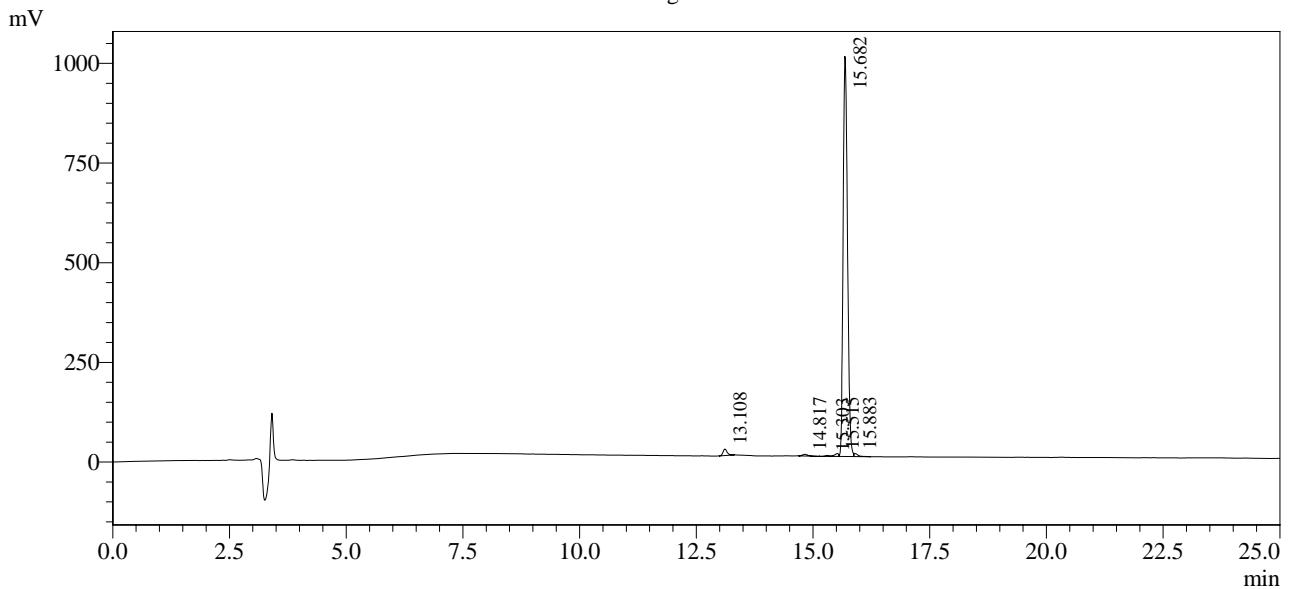

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.108	99500	16382	1.466
2	14.817	35114	4363	0.518
3	15.303	14101	2402	0.208
4	15.515	45594	7207	0.672
5	15.682	6546538	1003989	96.486
6	15.883	44129	7502	0.650
Total		6784975	1041844	100.000