


Mass Spectrum

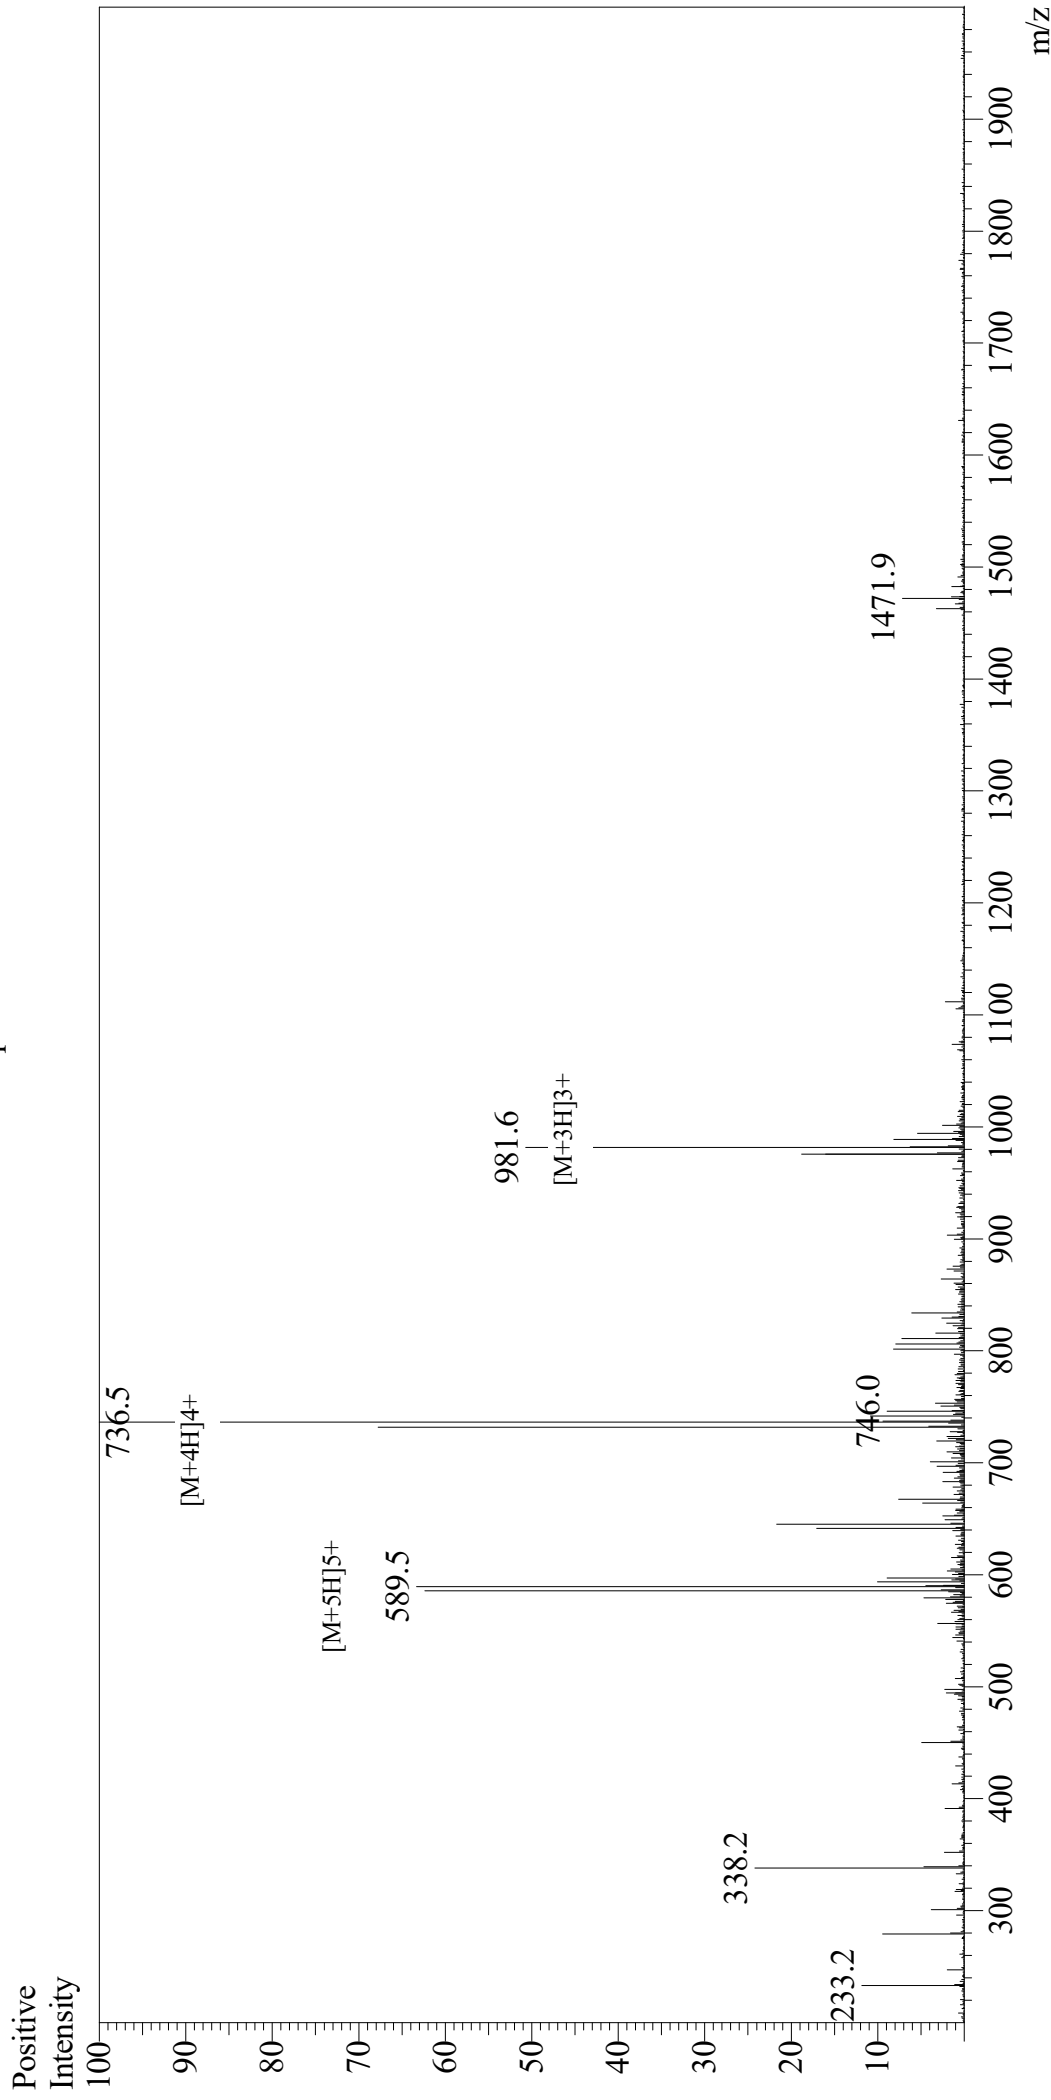

Sample Information

User : Gary
Month-Day Processed : 09/23/19
Time Processed : 11:19:06 AM
Injection Volume : 0.4
Sample Name : Alpha 1(I) Collagen (614-639), human
Cat No. : RP20424
Lot No. : E4966319I
Theoretical MW : 2942.20
Observed MW : 2942.0

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH