

Sample Name : N-Boc-Phe-Leu-Phe-Leu-Phe
 Cat. No. : RP12950
 Lot. No. : PE5181707

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
10.00	Pumps	Pump B Conc.	35	
35.00	Pumps	Pump B Conc.	95	
41.00	Pumps	Pump B Conc.	95	
41.01	Pumps	Pump B Conc.	5	
50.00	Pumps	Pump B Conc.	5	
50.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

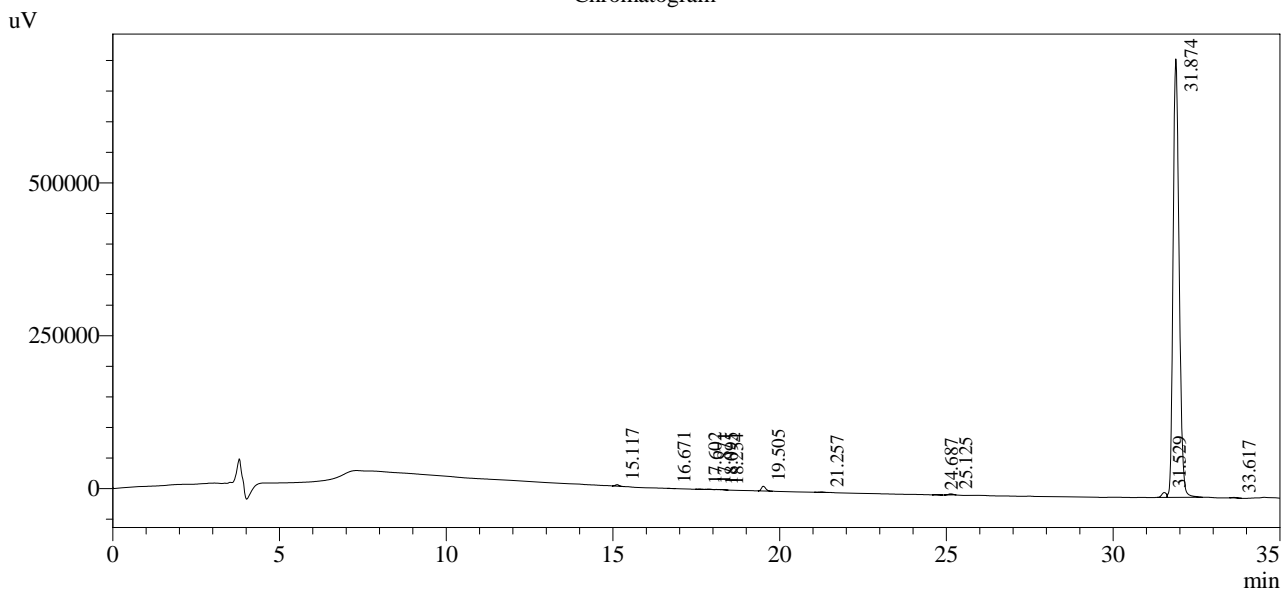

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.117	19757	2445	0.213
2	16.671	1088	110	0.012
3	17.602	2746	314	0.030
4	17.871	5809	746	0.063
5	18.095	1014	190	0.011
6	18.254	1753	243	0.019
7	19.505	69394	7772	0.749
8	21.257	6395	622	0.069
9	24.687	2479	307	0.027
10	25.125	17237	1751	0.186
11	31.529	76456	7967	0.825
12	31.874	9050194	717053	97.694
13	33.617	9483	895	0.102
Total		9263803	740415	100.000