

Sample Name :GRGDSPC
 Cat. No. : RP20283
 Lot. No. : E602620C
 Time Processed: 16:08:11
 Month-Day-Year Processed :12/03/2019
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	0
25.00	Pumps	Pump A B.Conc	50
25.01	Pumps	Pump A B.Conc	95
29.00	Pumps	Pump A B.Conc	95
29.01	Pumps	Pump A B.Conc	15
34.00	Pumps	Pump A B.Conc	15
34.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

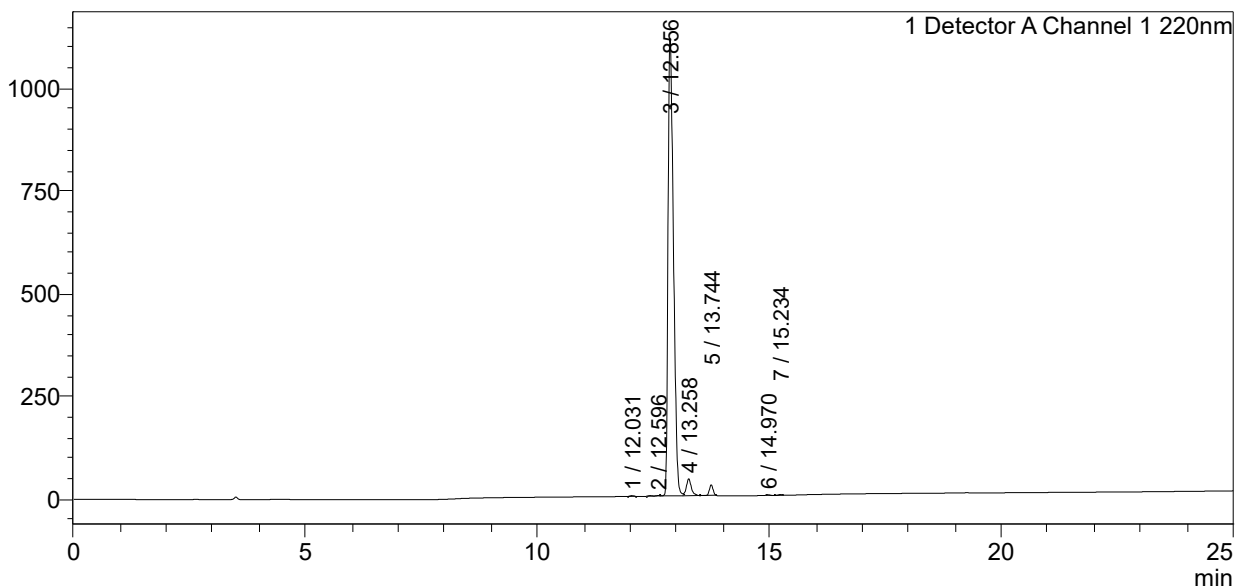

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.031	6978	1558	0.073
2	12.596	9588	1053	0.100
3	12.856	9077167	1114148	95.003
4	13.258	311638	40885	3.262
5	13.744	134972	25141	1.413
6	14.970	4983	1218	0.052
7	15.234	9326	1746	0.098
Total		9554651	1185749	100.000