

Sample Name : β -Amyloid (1-40)
 Cat. No. : RP20528
 Lot. No. : E49426191
 Time Processed : 12:28:17
 Month-Day-Year Processed : 10/01/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

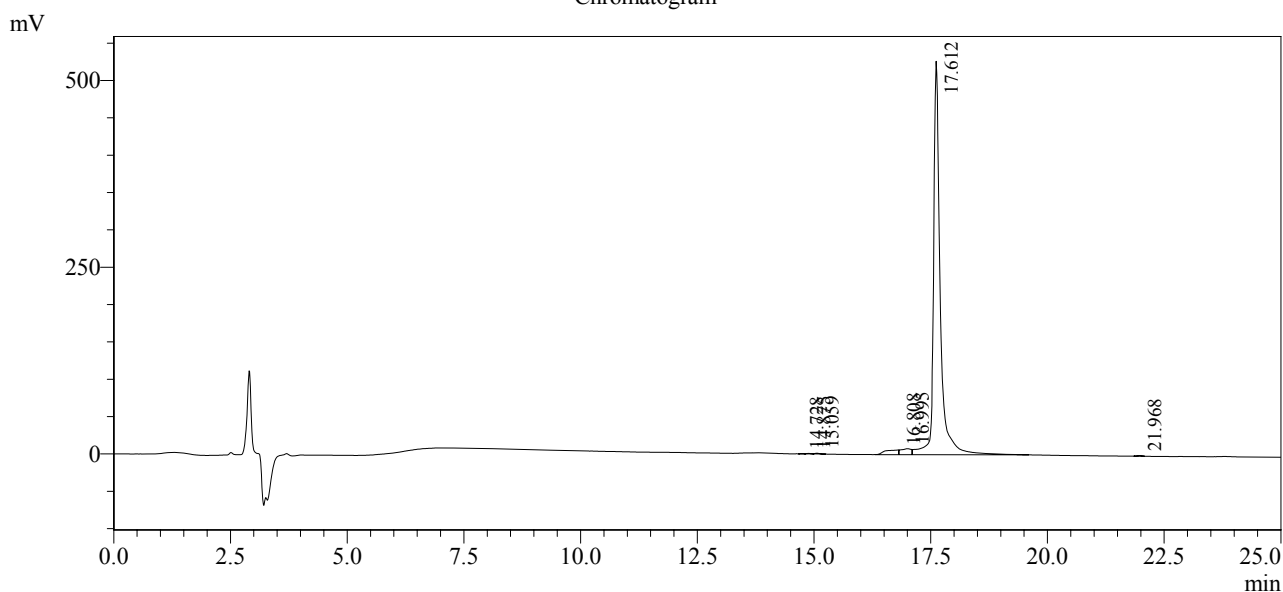

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.728	1265	228	0.023
2	14.875	3584	670	0.064
3	15.059	6648	1037	0.119
4	16.808	125992	6256	2.260
5	16.995	122231	7992	2.192
6	17.612	5301814	526863	95.088
7	21.968	3446	540	0.062
8	25.560	10741	1394	0.193
Total		5575721	544980	100.000