

Sample Name : Calcitonin Gene Related Peptide (CGRP) (8-37), human  
 Cat No. : RP11089  
 Lot No. : E9306120D  
 Time Processed : 9:24:49  
 Month-Day-Year Processed : 04/11/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>  
 Column : Alltima™ C18 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

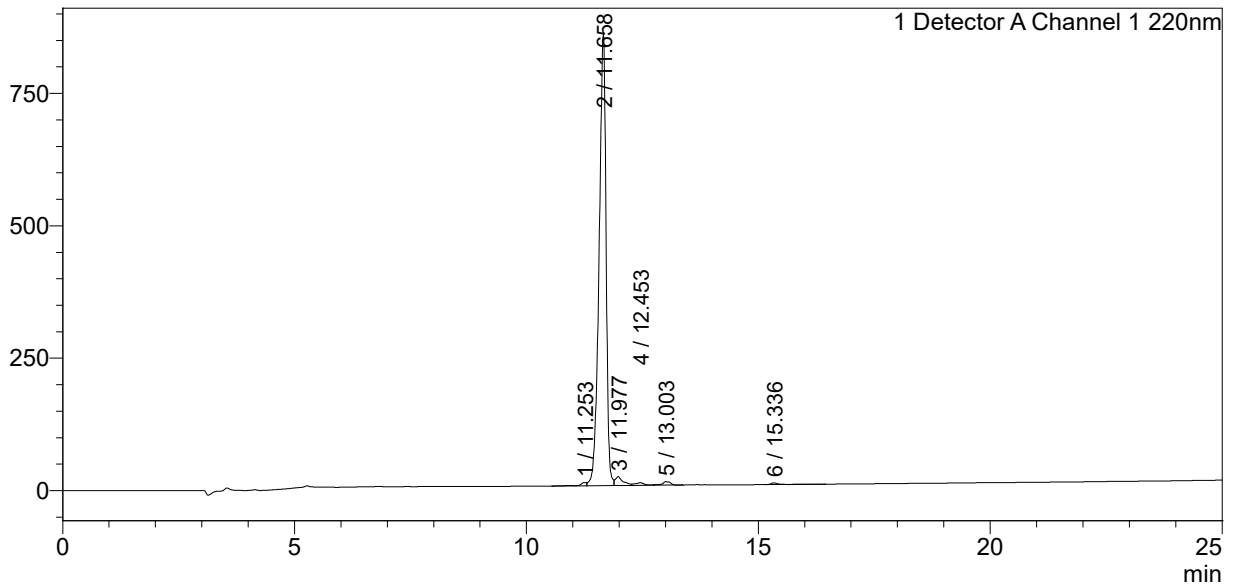

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.253	62236	6244	0.665
2	11.658	8919621	852750	95.258
3	11.977	194281	16862	2.075
4	12.453	73728	5072	0.787
5	13.003	83034	6754	0.887
6	15.336	30700	3114	0.328
Total		9363601	890794	100.000