

Sample Name :Calcitonin Gene Related Peptide (CGRP), rat
Cat No. :RP11095
Lot No. :E5231221I
Time Processed : 14:02:09
Month-Day-Year Processed : 09/20/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

| Time | Module | Command | Value |
|-------|------------|---------------|-------|
| 0.01 | Pumps | Pump A B.Conc | 5 |
| 25.00 | Pumps | Pump A B.Conc | 65 |
| 25.01 | Pumps | Pump A B.Conc | 95 |
| 27.00 | Pumps | Pump A B.Conc | 95 |
| 27.01 | Pumps | Pump A B.Conc | 5 |
| 35.00 | Pumps | Pump A B.Conc | 5 |
| 35.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

mV

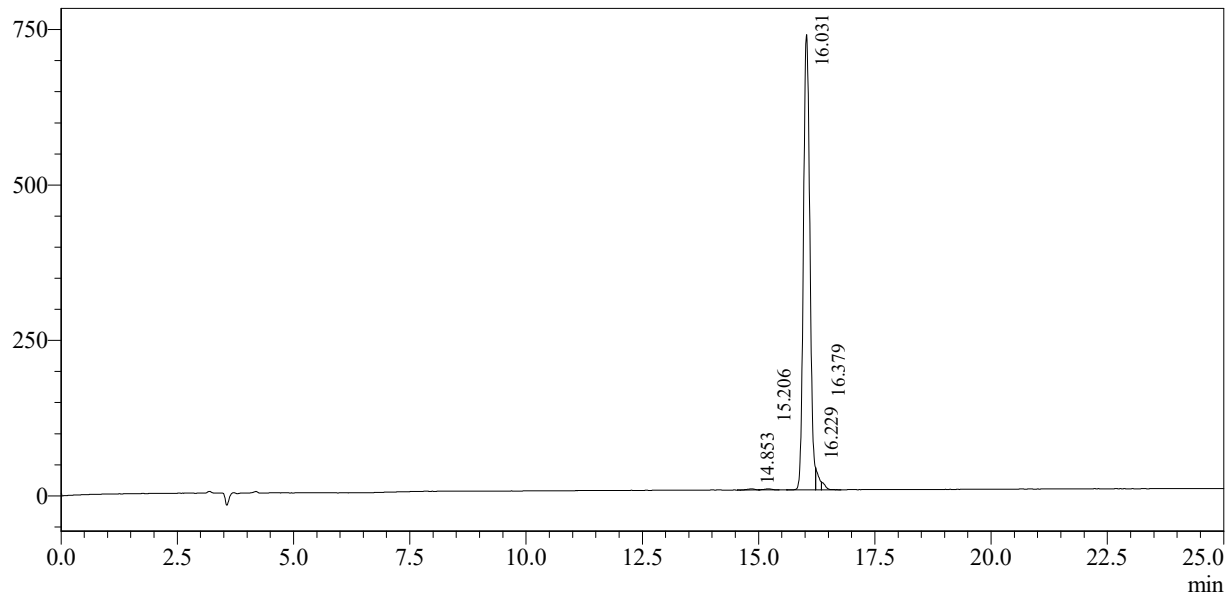

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area % |
|-------|-----------|---------|--------|---------|
| 1 | 14.853 | 20316 | 1698 | 0.277 |
| 2 | 15.206 | 20334 | 1630 | 0.277 |
| 3 | 16.031 | 7066250 | 719600 | 96.348 |
| 4 | 16.229 | 161978 | 38423 | 2.209 |
| 5 | 16.379 | 65214 | 11707 | 0.889 |
| Total | | 7334091 | 773058 | 100.000 |