

Sample Name :  $\gamma$ -2-MSH (41-58), amide  
 Cat No. : RP20307  
 Lot No. : E9801020J  
 Time Processed: 0:41:49  
 Year-Month-Day: 2020/11/4

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min

<<Detector A>>  
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
33.00	Pumps	Solvent B Conc.	5	
33.01	Controller	Stop		

<<Column Performance>>

<Detector A>  
 Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010015

<Chromatogram>

mV

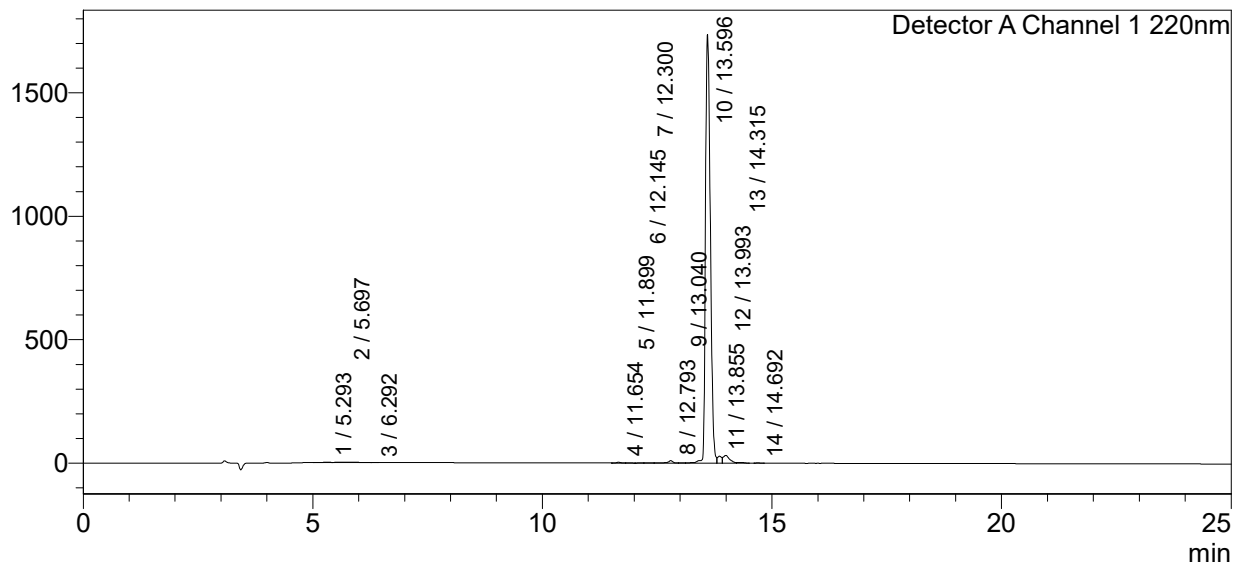

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.293	10511	1334	0.077
2	5.697	23846	668	0.176
3	6.292	1768	226	0.013
4	11.654	21031	2891	0.155
5	11.899	3350	600	0.025
6	12.145	2955	476	0.022
7	12.300	7981	883	0.059
8	12.793	77348	9639	0.570
9	13.040	6824	907	0.050
10	13.596	12915932	1735365	95.110
11	13.855	174351	27608	1.284
12	13.993	303278	31330	2.233
13	14.315	25144	2749	0.185
14	14.692	5676	1089	0.042

Peak#	Ret. Time	Area	Height	Area%
Total		13579996	1815765	100.000