

Sample Name :Thrombin Receptor Agonist  
 Cat No. :RP10623  
 Lot No. :E4744019I  
 Time Processed :7:34:15  
 Month-Day-Year Processed :09/18/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ17010508

### <Chromatogram>

mV

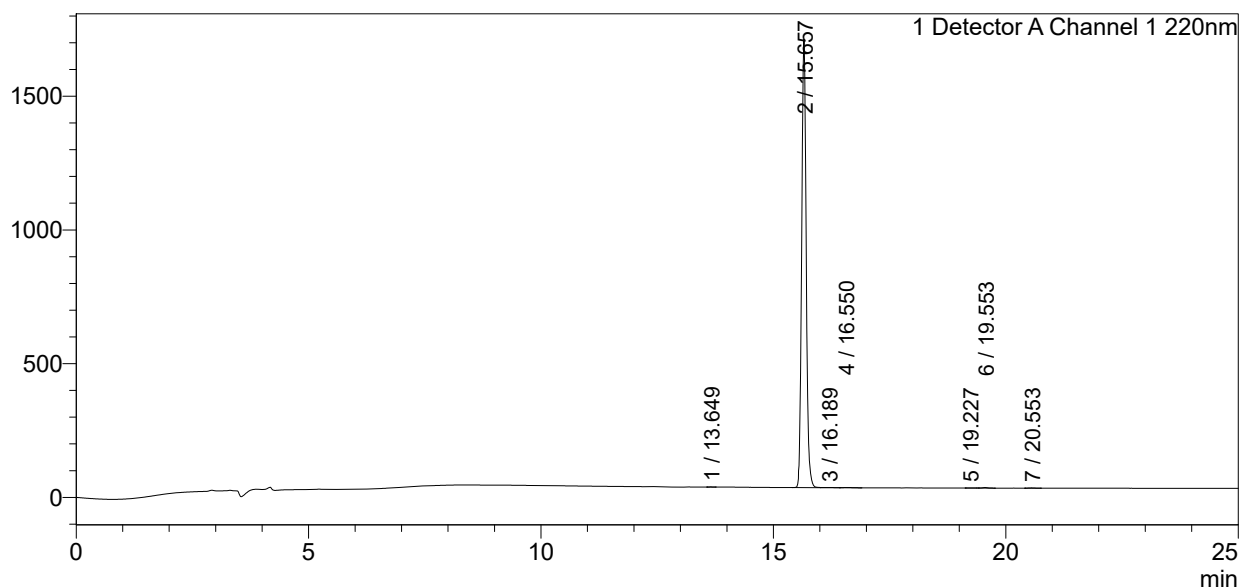

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.649	1891	369	0.017
2	15.657	11338362	1675749	99.595
3	16.189	12245	871	0.108
4	16.550	8997	622	0.079
5	19.227	2678	402	0.024
6	19.553	14231	2018	0.125
7	20.553	6081	808	0.053
Total		11384485	1680839	100.000