

Sample Name :hgp100(25-33)

Cat. No. : RP20344 Lot. No. : PE6561712

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

<Chromatogram>

mV

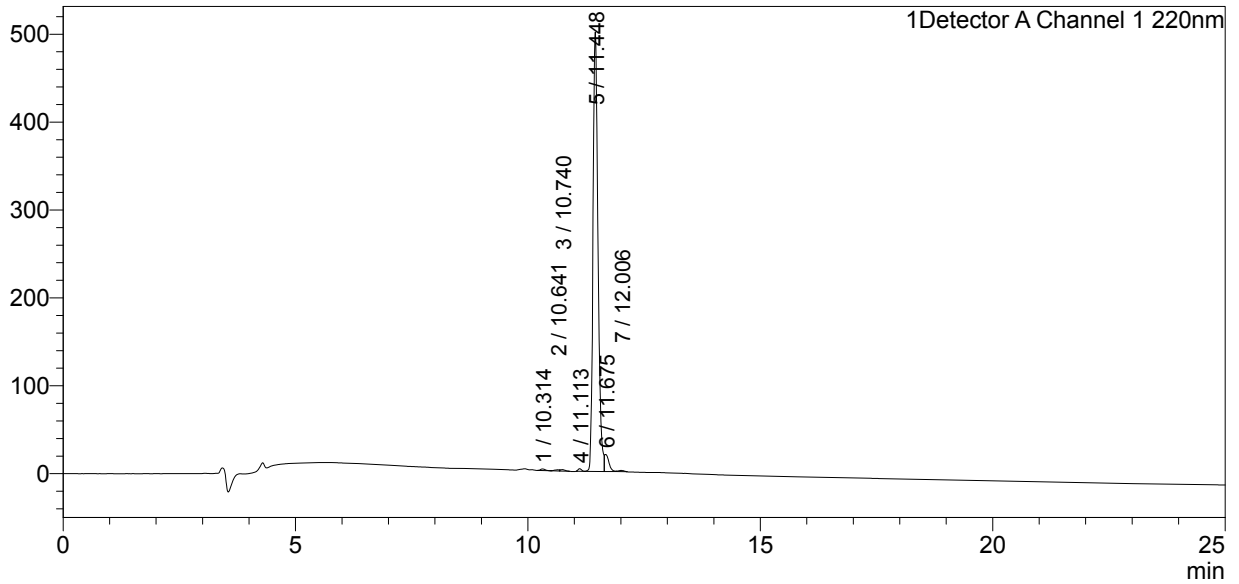

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.314	12927	1838	0.331
2	10.641	9574	1284	0.245
3	10.740	11056	1592	0.283
4	11.113	14537	2840	0.372
5	11.448	3721216	499871	95.277
6	11.675	125507	19363	3.213
7	12.006	10883	1318	0.279
Total		3905699	528107	100.000