

Sample Name: Phe-Met-Arg-Phe
 Cat No. : RP10814
 Lot No. : E4779619I
 Time Processed: 1:17:40 PM
 Month-Day-Year Processed :09/22/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

mV

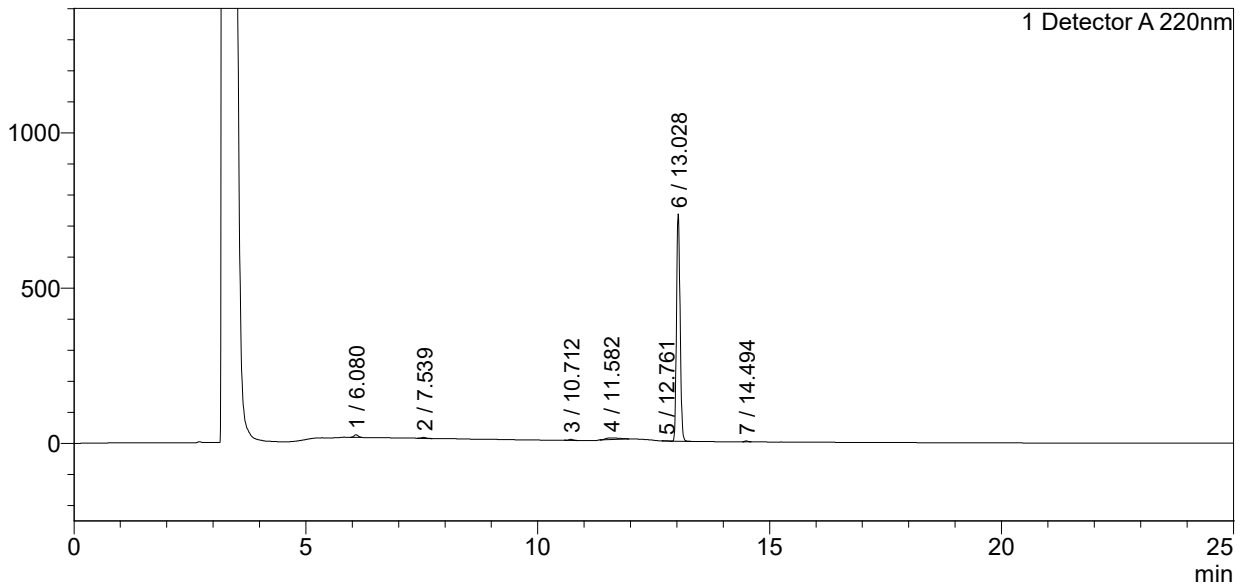

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.080	49313	7984	1.180
2	7.539	18390	2756	0.440
3	10.712	20638	3355	0.494
4	11.582	95469	4827	2.284
5	12.761	2128	441	0.051
6	13.028	3980569	731678	95.239
7	14.494	13044	2652	0.312
Total		4179550	753693	100.000