

Sample Name : Moth Cytochrome C (MCC) (88-103)
 Cat No.: RP12808
 Lot No.: E4886219I
 Time Processed: 7:25:11
 Month-Day-Year Processed: 09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010014

<Chromatogram>

mV

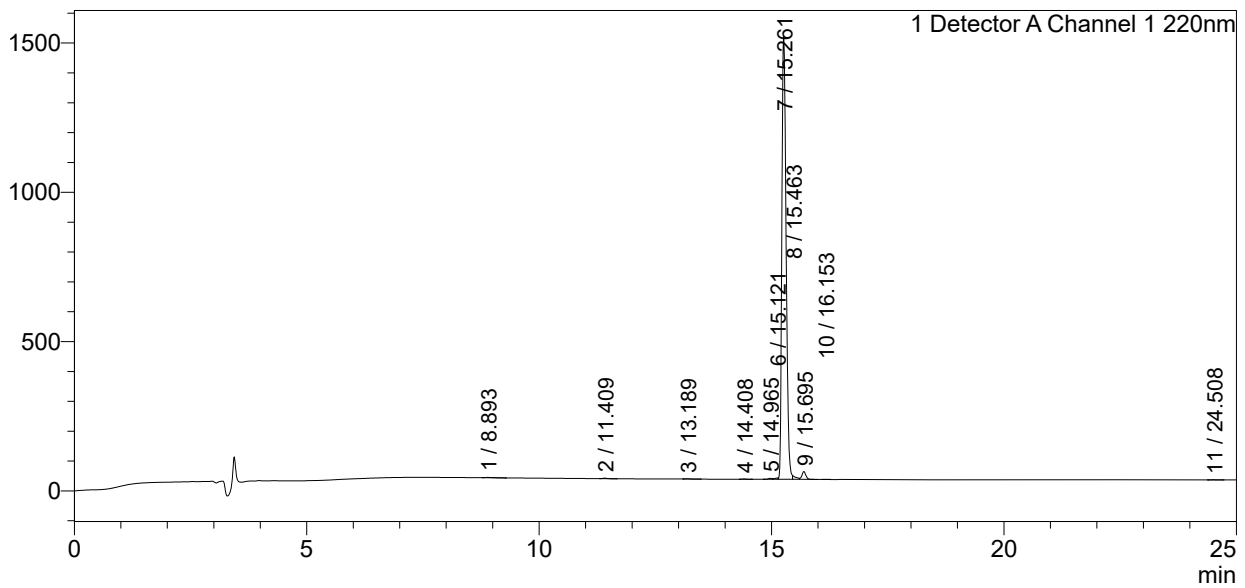

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.893	12245	1202	0.126
2	11.409	11198	1995	0.115
3	13.189	4531	782	0.047
4	14.408	6465	1188	0.066
5	14.965	17252	3019	0.177
6	15.121	22238	4206	0.228
7	15.261	9447676	1484263	97.016
8	15.463	61249	12095	0.629
9	15.695	150743	26038	1.548
10	16.153	1408	303	0.014
11	24.508	3273	418	0.034
Total		9738279	1535509	100.000