

Sample Name : Calcitonin, eel
 Cat. No. : RP12786
 Lot. No. : E4009420G
 Time Processed : 14:11:01
 Month-Day-Year Processed : 07/17/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

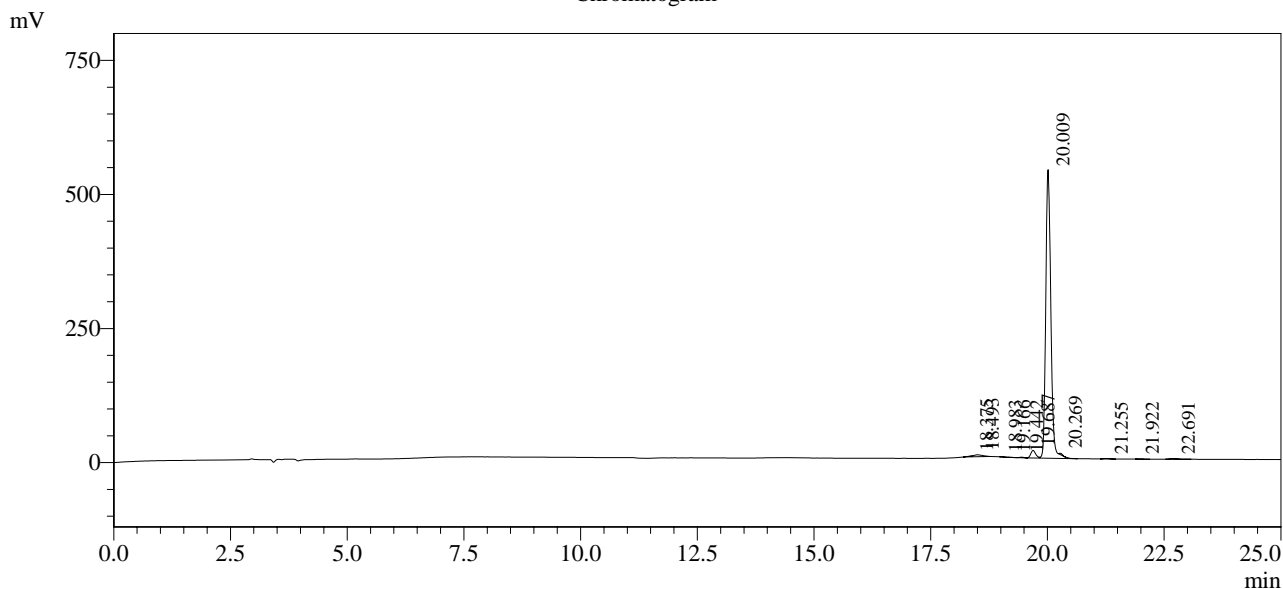

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	18.375	11770	1930	0.274
2	18.493	46607	3588	1.086
3	18.983	665	46	0.016
4	19.166	2142	256	0.050
5	19.442	6930	1101	0.162
6	19.687	104581	14208	2.438
7	20.009	4084878	538072	95.219
8	20.269	10798	2263	0.252
9	21.255	6947	827	0.162
10	21.922	1360	182	0.032
11	22.691	13302	1189	0.310
Total		4289980	563663	100.000