

Sample Name :[Asp371]-Tyrosinase (369-377), human
 Cat. No. : RP10270
 Lot. No. : E7532520B
 Time Processed :9:45:56
 Month-Day-Year :02/14/2020


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GR11010440

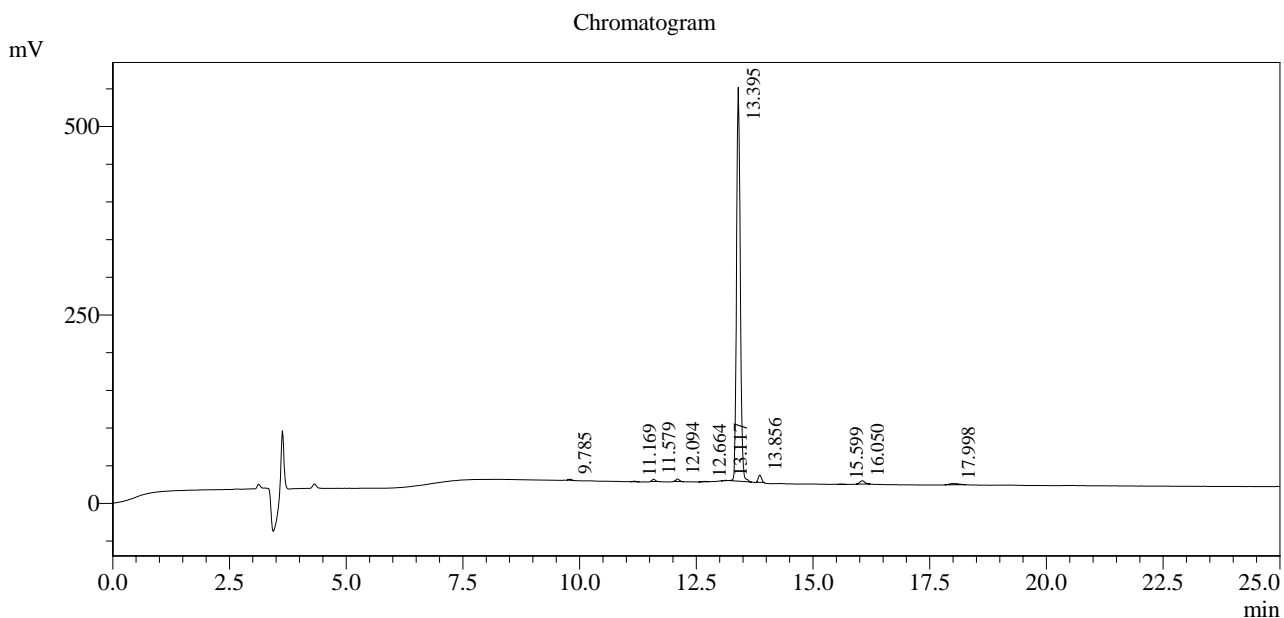

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.785	5272	1273	0.172
2	11.169	3765	747	0.123
3	11.579	14771	2984	0.483
4	12.094	17341	3412	0.567
5	12.664	2929	522	0.096
6	13.117	1976	425	0.065
7	13.395	2910028	522714	95.188
8	13.856	45863	9536	1.500
9	15.599	1867	366	0.061
10	16.050	31471	4273	1.029
11	17.998	21859	1581	0.715
Total		3057142	547833	100.000