

Sample Name :Cortistatin 14, human, rat
 Cat No. :RP10972
 Lot No. :E2342820A
 Time Processed :23:58:30
 Month-Day-Year Processed :01/21/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

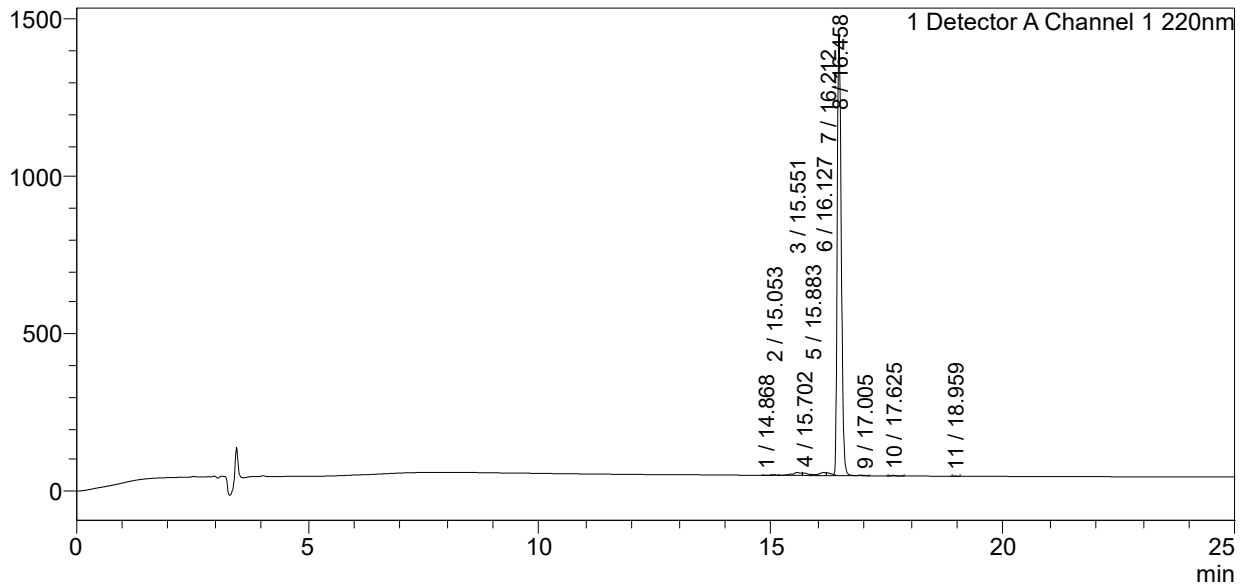

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.868	1948	412	0.022
2	15.053	11691	2342	0.131
3	15.551	122335	9750	1.369
4	15.702	67248	7704	0.753
5	15.883	21298	3394	0.238
6	16.127	90782	9873	1.016
7	16.212	60957	8524	0.682
8	16.458	8539973	1406238	95.572
9	17.005	3576	812	0.040
10	17.625	13486	2169	0.151
11	18.959	2375	439	0.027
Total		8935671	1451655	100.000