


Mass Spectrum

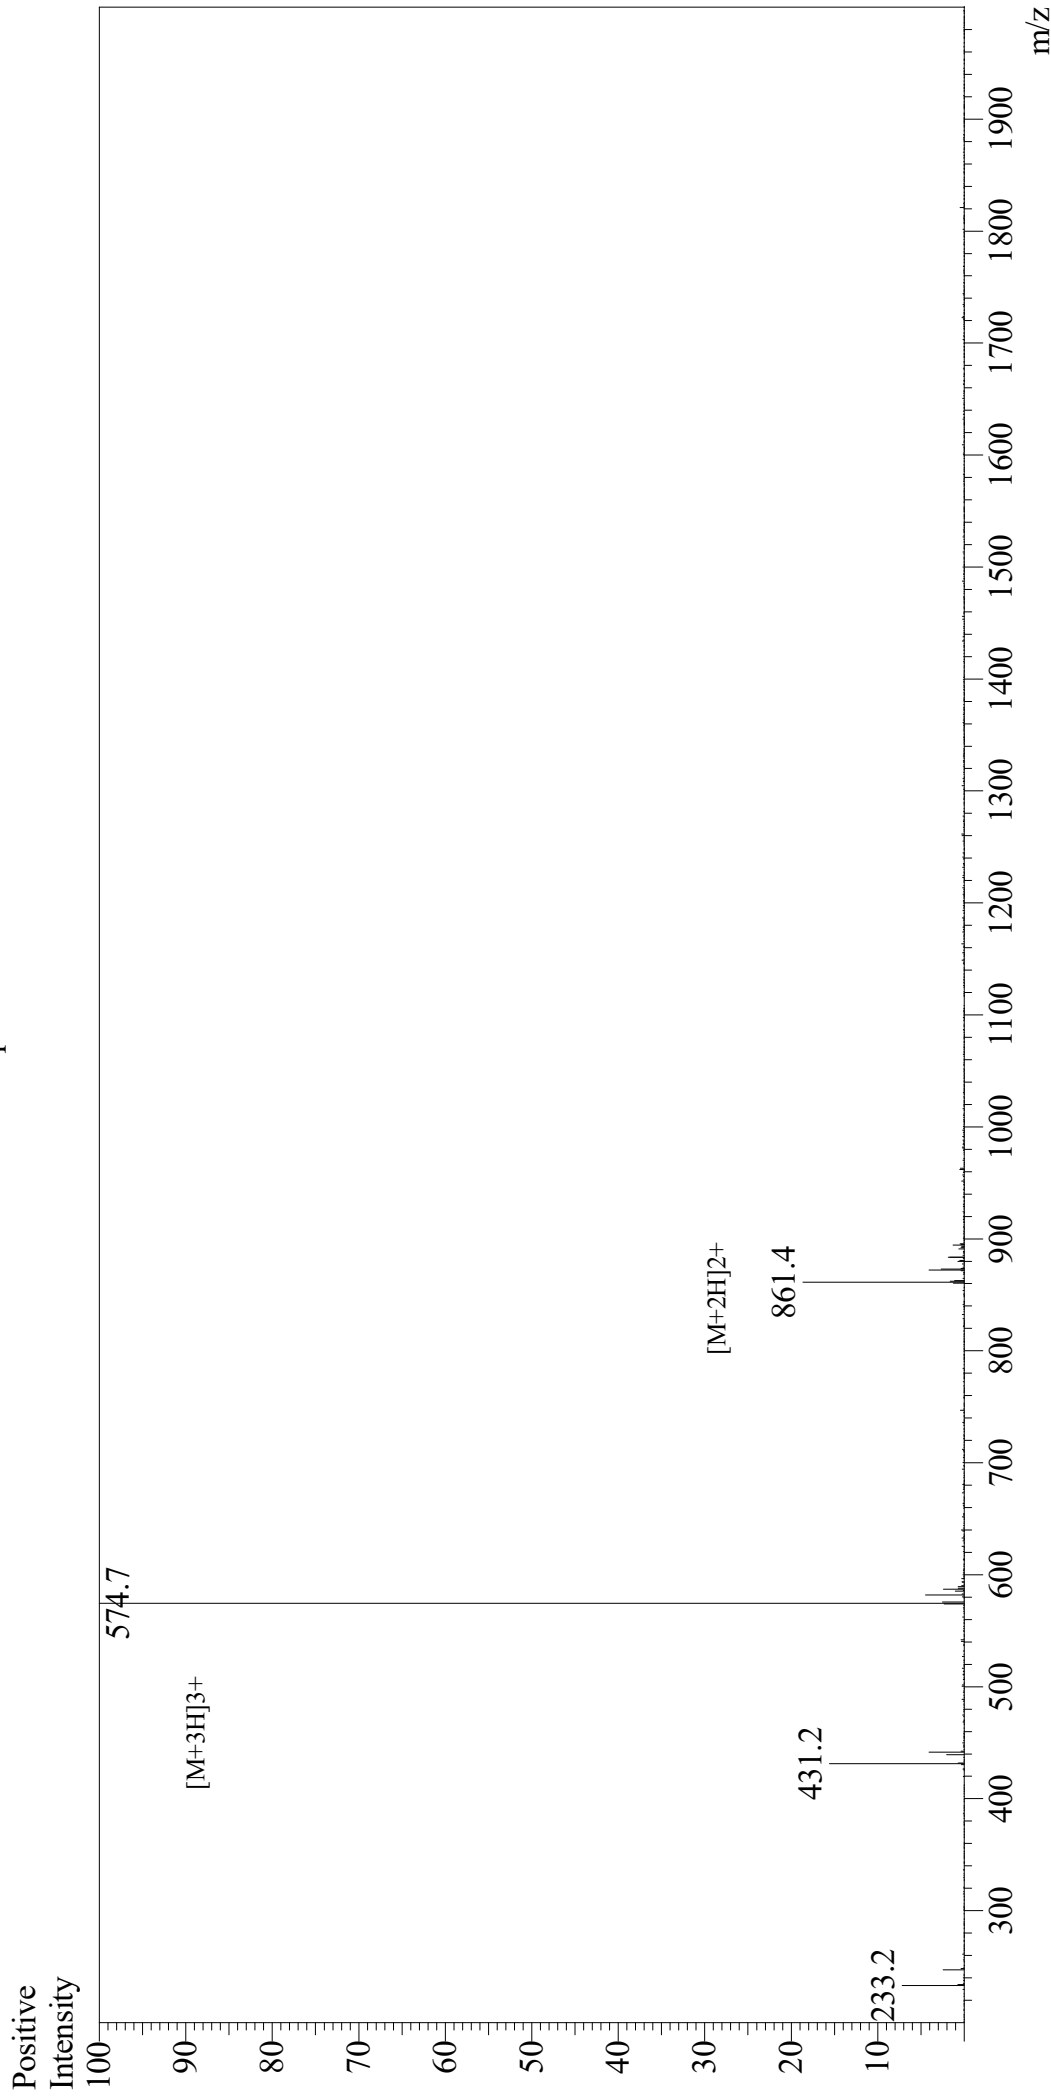

Sample Information

User : Gary
Month-Day Processed : 01/21/20
Time Processed : 06:43:51 PM
Injection Volume : 0.4
Sample Name : Cortistatin 14, human, rat
Cat No. : RP10972
Lot No. : E2342820A
Theoretical MW : 1721.01
Observed MW : 1721.1

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200