

Sample Name: IRBP(161-180)
 Cat No. : RP11841
 Lot No. : E4879319I
 Time Processed: 11:28:11 AM
 Month-Day-Year Processed :09/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010325

<Chromatogram>

mV

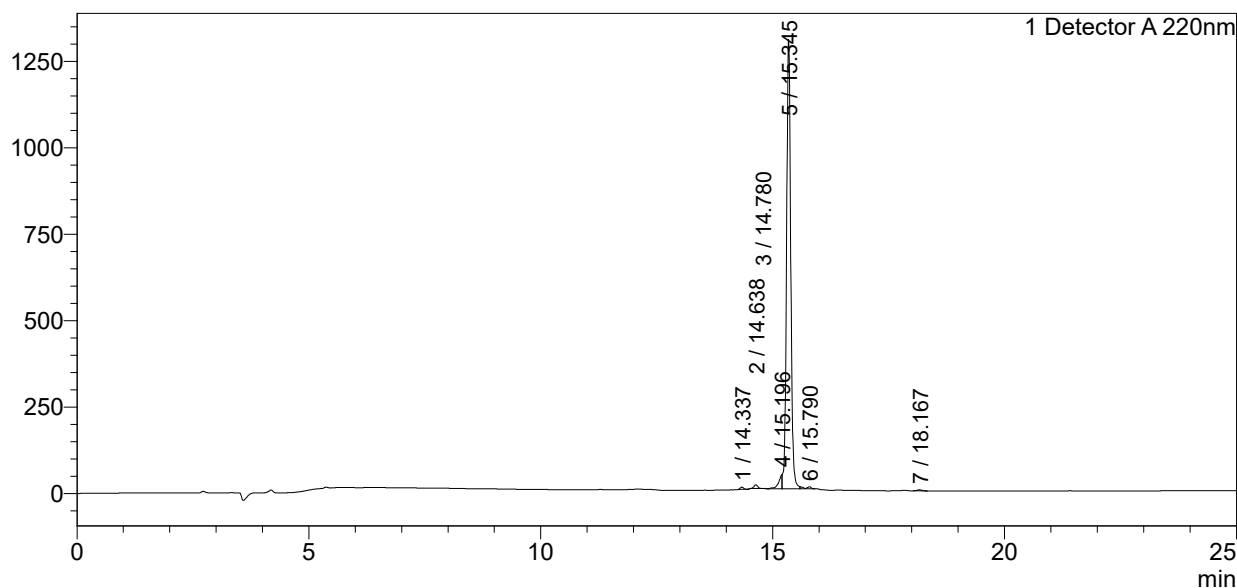

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.337	31911	6862	0.371
2	14.638	62097	10677	0.722
3	14.780	2074	553	0.024
4	15.196	202317	39607	2.351
5	15.345	8228424	1300555	95.609
6	15.790	59087	5975	0.687
7	18.167	20433	2957	0.237
Total		8606343	1367186	100.000