

Sample Name :Rhodopsin Epitope Tag  
 Cat No. :RP20400  
 Lot No. :E5697919F  
 Time Processed :4:06:19 PM  
 Month-Day-Year Processed :06/30/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010141

### <Chromatogram>

mV

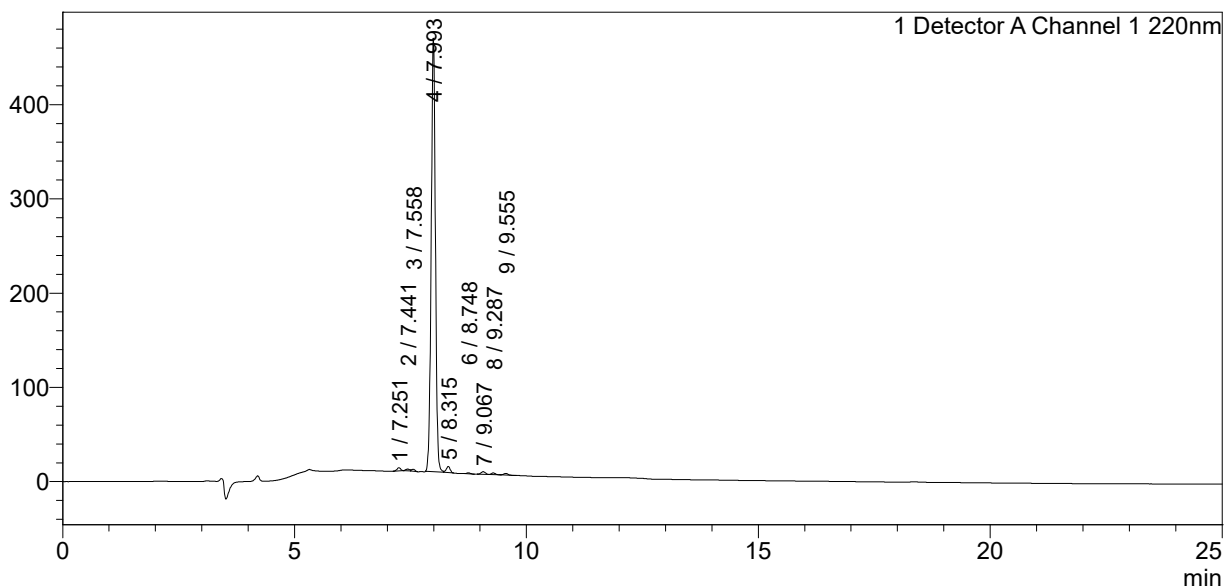

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.251	18308	3375	0.604
2	7.441	11948	1865	0.394
3	7.558	10238	2163	0.338
4	7.993	2912876	460039	96.072
5	8.315	35965	6385	1.186
6	8.748	5578	1058	0.184
7	9.067	17231	2805	0.568
8	9.287	9301	1702	0.307
9	9.555	10515	1796	0.347
Total		3031960	481189	100.000