

Sample Name: Somatostatin 28 (1-14)
 Cat No. : RP10230
 Lot No. : E3955320D
 Time Processed: 5:21:25 PM
 Month-Day-Year Processed :04/14/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

mV

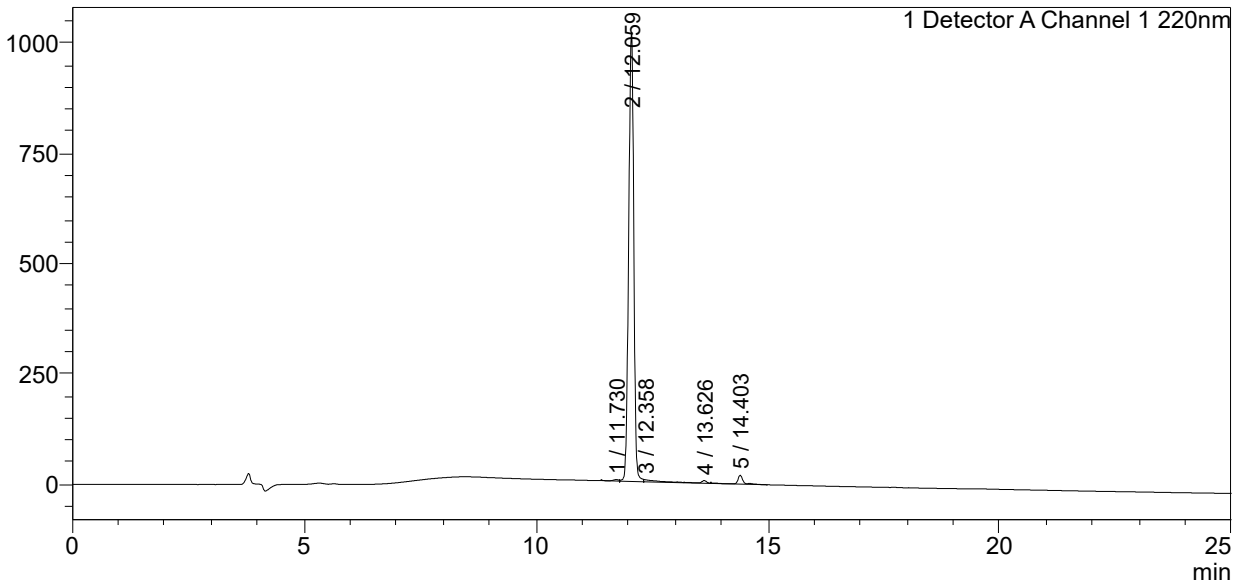

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.730	28007	3245	0.348
2	12.059	7713887	1001733	95.804
3	12.358	93505	4710	1.161
4	13.626	52317	5808	0.650
5	14.403	164057	19905	2.038
Total		8051773	1035402	100.000