

Sample Name :  $\beta$ -Amyloid (1-9)  
 Cat No.: RP20160  
 Lot No.:E4841619I  
 Time Processed :13:29:19  
 Month-Day-Year Processed :09/30/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

### <Chromatogram>

mV

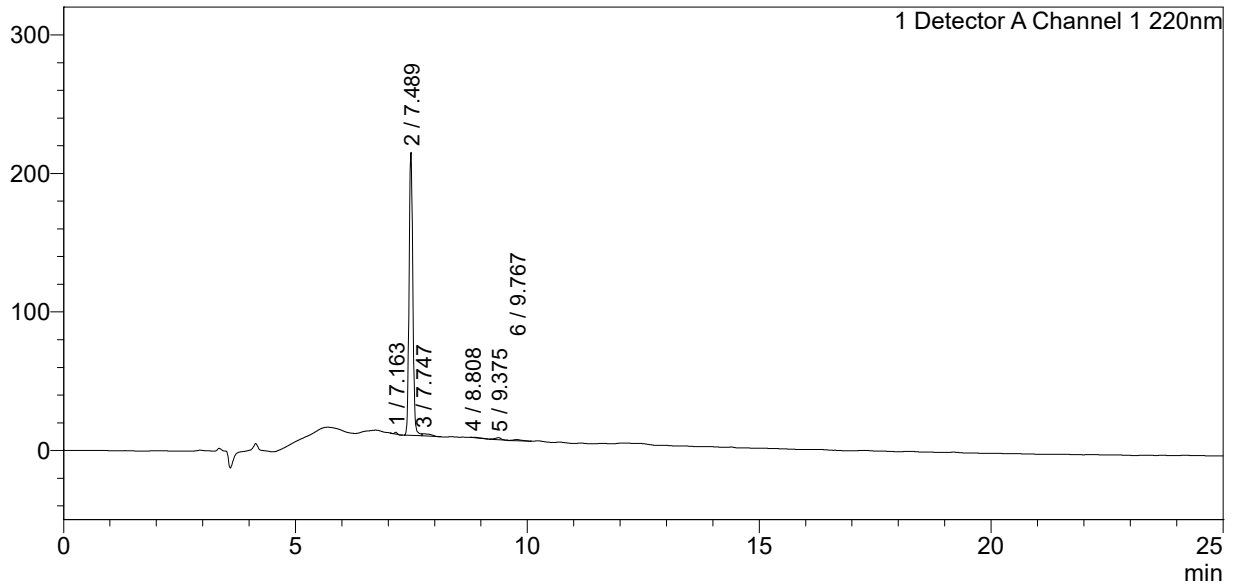

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.163	4180	1288	0.350
2	7.489	1140219	204209	95.597
3	7.747	21720	1492	1.821
4	8.808	3438	127	0.288
5	9.375	13540	1529	1.135
6	9.767	9635	756	0.808
Total		1192733	209401	100.000