

Sample Name :InsB 9-23  
 Cat. No. :RP20391  
 Lot. No. :PE1561801

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

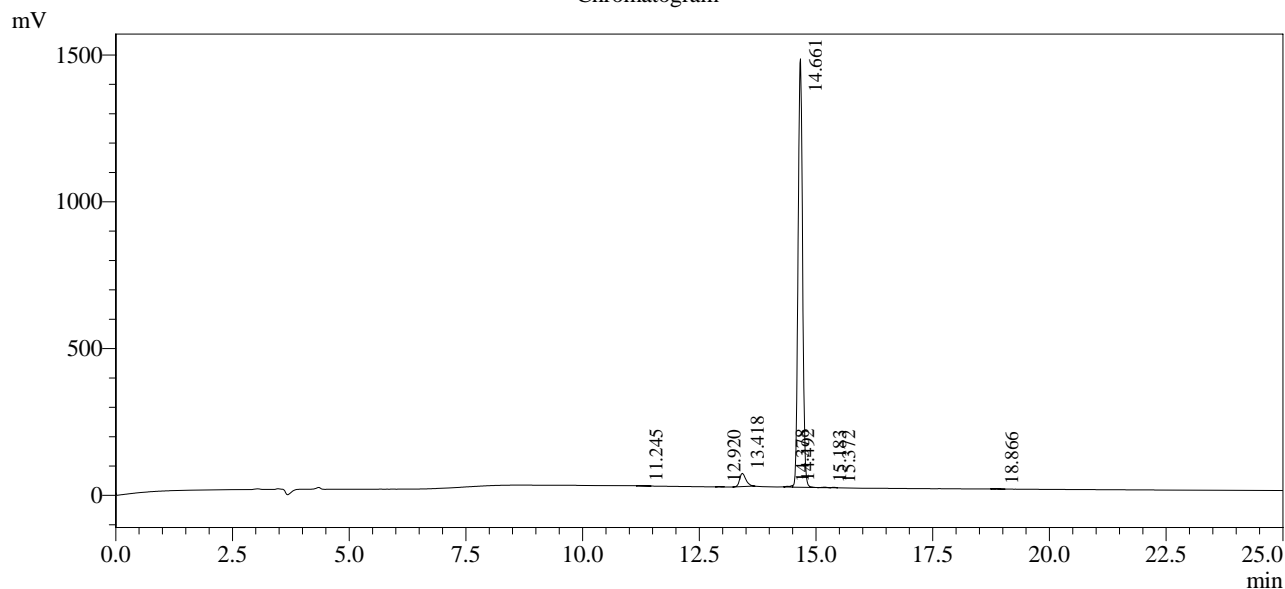

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.245	8921	1491	0.087
2	12.920	2399	437	0.023
3	13.418	422500	45074	4.109
4	14.378	13514	2488	0.131
5	14.492	16295	5325	0.158
6	14.661	9791817	1459228	95.238
7	15.183	12277	1730	0.119
8	15.372	8455	1670	0.082
9	18.866	5215	683	0.051
Total		10281392	1518126	100.000