

Sample Name :LAH4
 Cat No.: RP20096
 Lot No.: PE0261905
 Time Processed:9:03:47
 Month-Day-Year Processed:05/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

<Chromatogram>

mV

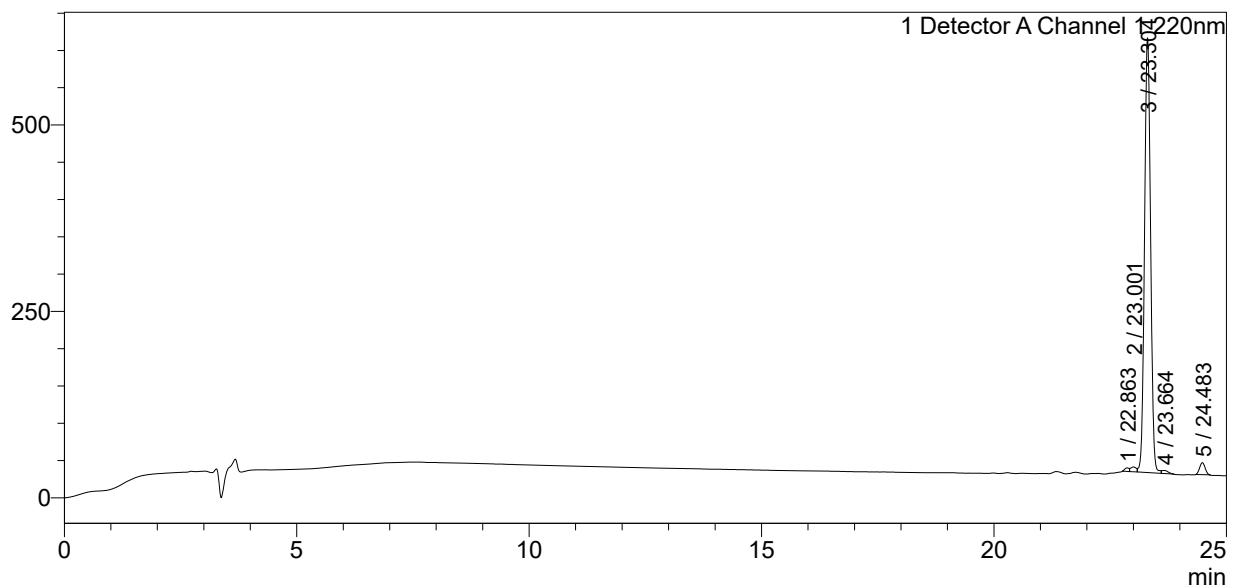

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	22.863	31178	4704	0.566
2	23.001	54845	6535	0.996
3	23.304	5250320	582914	95.386
4	23.664	37467	4100	0.681
5	24.483	130484	16072	2.371
Total		5504295	614326	100.000