

Sample Name :Indolicidin
 Cat No. :RP11242
 Lot No. :E5914020C
 Time Processed :8:22:12
 Month-Day-Year Processed :03/27/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

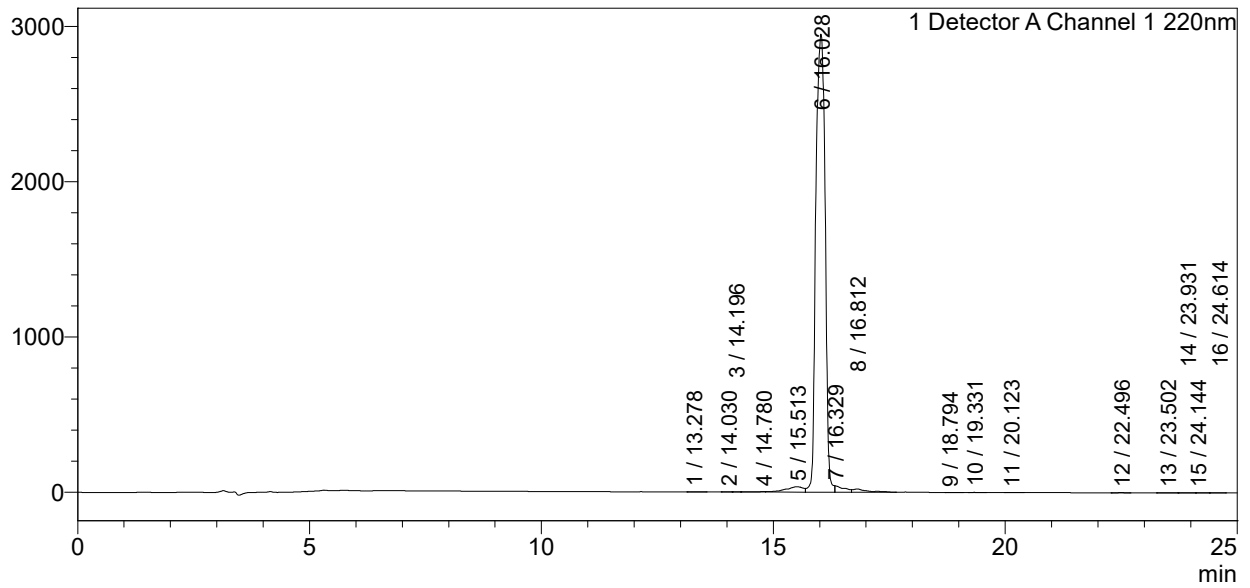

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.278	8815	675	0.021
2	14.030	1969	248	0.005
3	14.196	2443	234	0.006
4	14.780	42181	2518	0.098
5	15.513	904999	34832	2.113
6	16.028	40856983	2949448	95.385
7	16.329	561588	41407	1.311
8	16.812	425693	20399	0.994
9	18.794	3689	288	0.009
10	19.331	7329	913	0.017
11	20.123	4339	440	0.010
12	22.496	5171	548	0.012
13	23.502	3198	247	0.007
14	23.931	3178	214	0.007
15	24.144	1120	121	0.003

Peak#	Ret. Time	Area	Height	Area%
16	24.614	1210	107	0.003
Total		42833906	3052638	100.000