

Sample Name :Influenza Hemagglutinin (307-319)
 Cat No. :RP20087
 Lot No. :E3468120E
 Time Processed :10:09:21 AM
 Month-Day-Year Processed :05/30/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

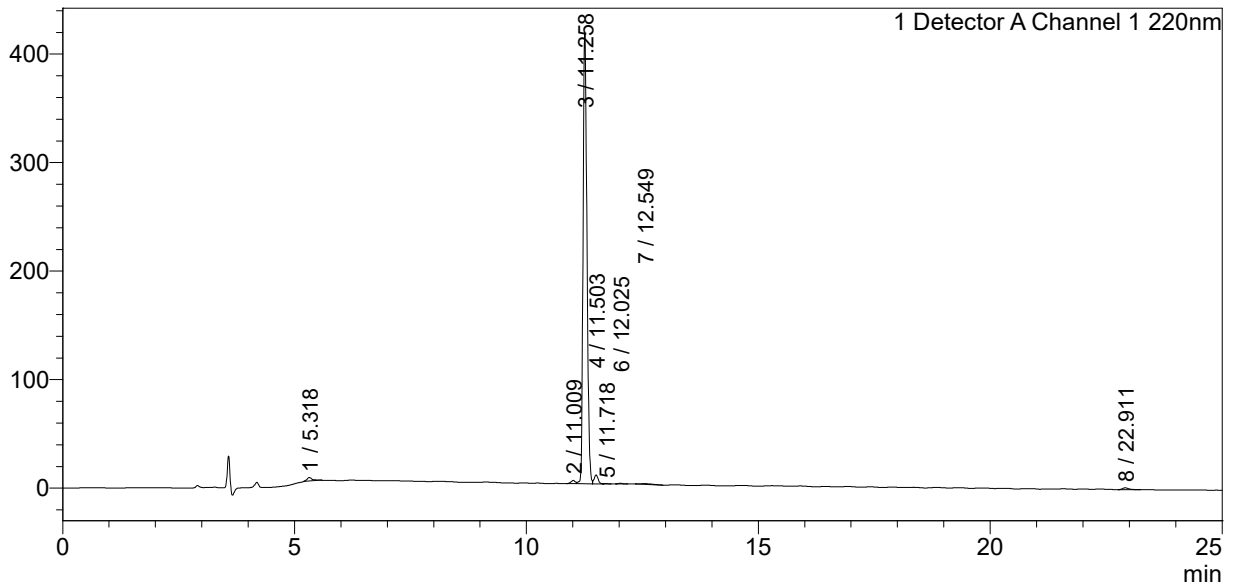

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.318	27514	3243	1.072
2	11.009	19616	3036	0.764
3	11.258	2438391	414462	95.021
4	11.503	49066	8244	1.912
5	11.718	1936	432	0.075
6	12.025	4329	759	0.169
7	12.549	10349	531	0.403
8	22.911	14972	1662	0.583
Total		2566173	432369	100.000