


Mass Spectrum

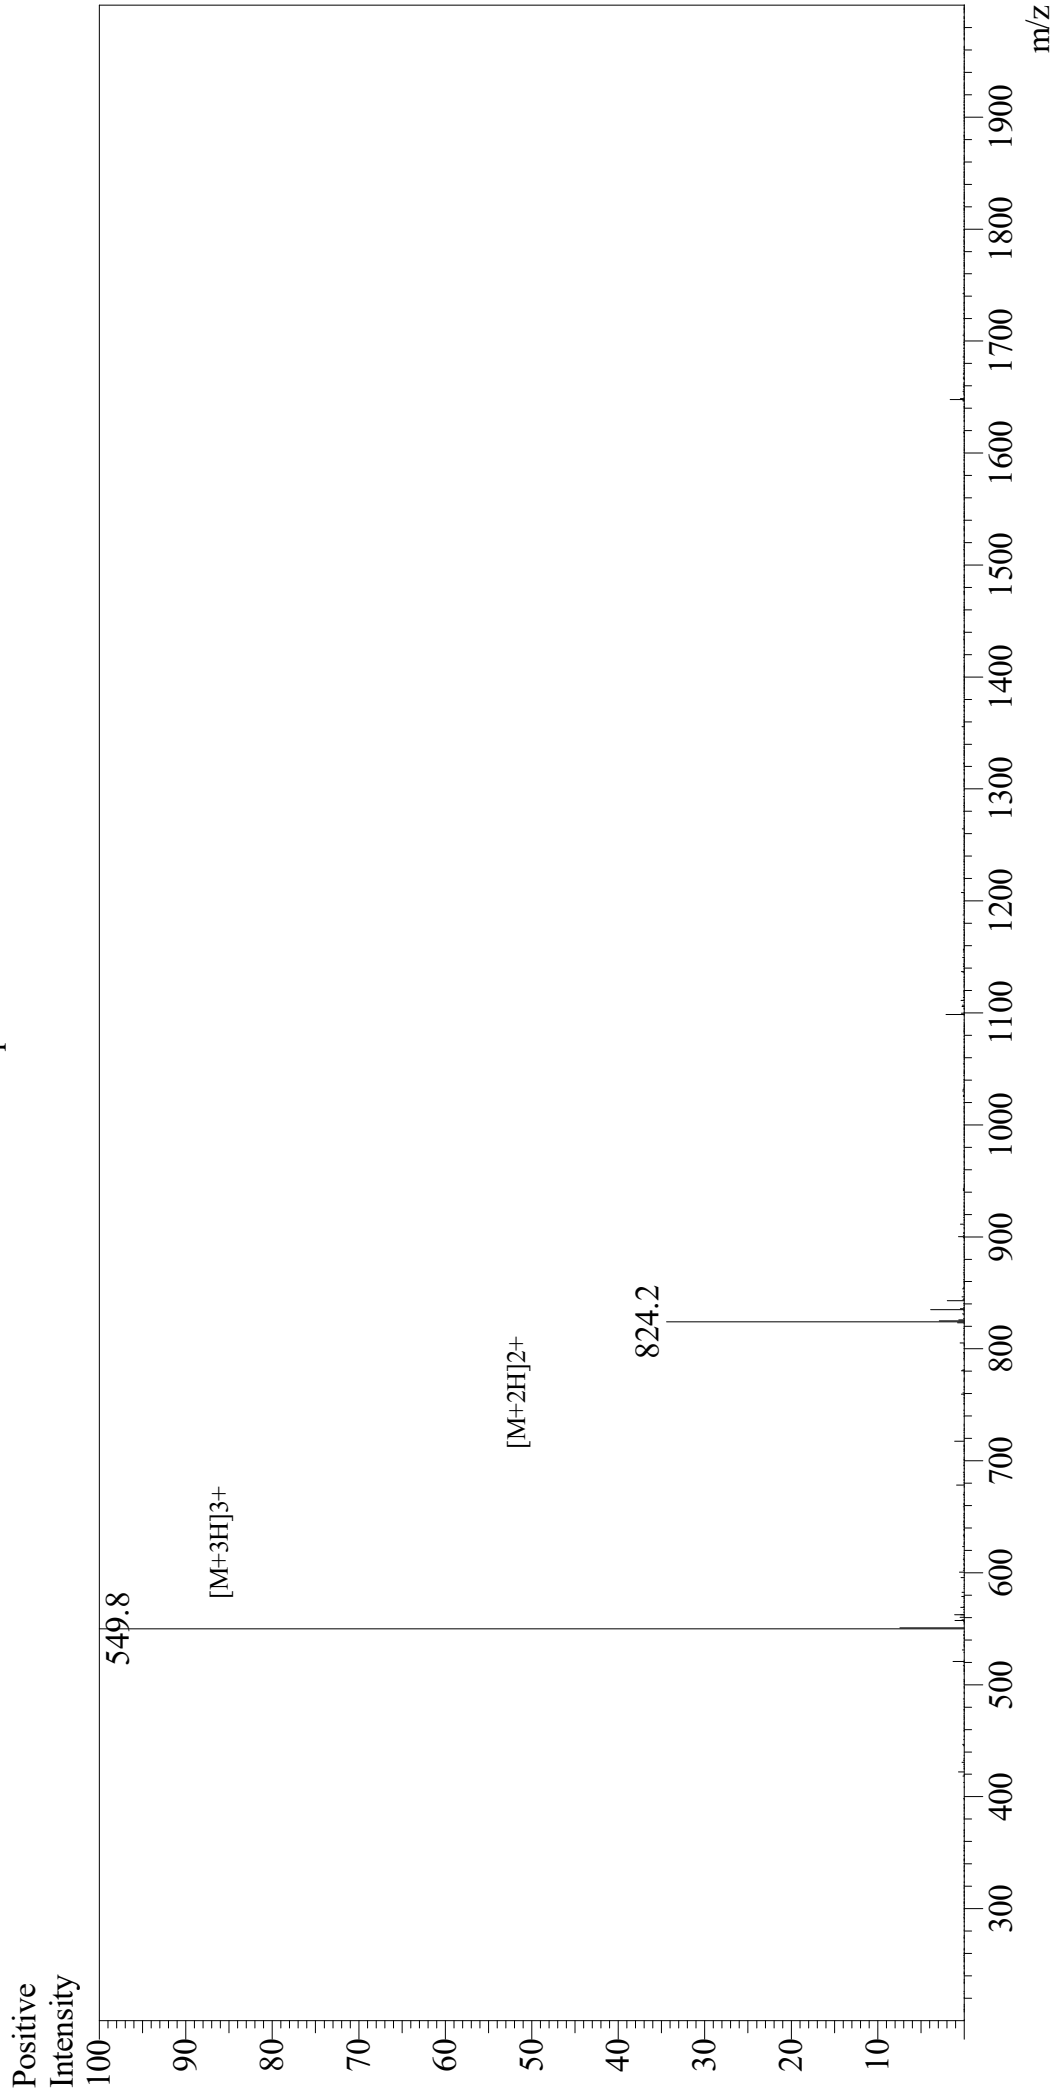

Sample Information

User : Gary
Month-Day Processed : 10/15/19
Time Processed : 05:57:35 PM
Injection Volume : 0.3
Sample Name : [Nle4, D-Phe7]- α -MSH, amide
Cat No. : RP10658
Lot No. : E6792819J
Theoretical MW : 1647.00
Observed MW : 1646.4

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200